


Operating Instructions

Indumax CLS50D/CLS50

Digital sensor with Memosens protocol or analog sensor

For inductive measurement of conductivity in liquids

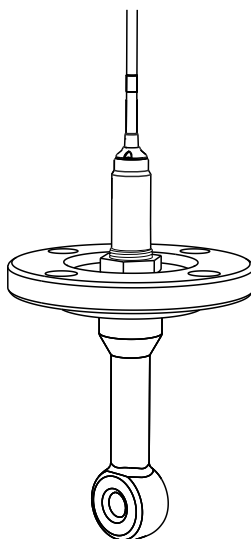

EU Declaration of Conformity

CLS50D-BA****

EU-Konformitätserklärung
EU-Declaration of Conformity
Déclaration UE de Conformité

Endress+Hauser 
People for Process Automation



Company **Endress+Hauser Conducta GmbH+Co. KG**
Dieselstraße 24, 70839 Gerlingen, Germany
erklärt als Hersteller in alleiniger Verantwortung, dass das Produkt
declares as manufacturer under sole responsibility, that the product
déclare sous sa seule responsabilité en qualité de fabricant que le produit

Product **Indumax**
CLS50D-BA****

Regulations den folgenden Europäischen Richtlinien entspricht:
conforms to following European Directives:
est conforme aux prescription des Directives Européennes suivantes :

EMC 2014/30/EU (L96/79)
ATEX 2014/34/EU (L96/309)

Standards angewandte harmonisierte Normen oder normative Dokumente:
applied harmonized standards or normative documents:
normes harmonisées ou documents normatifs appliqués :

EN 61326-1	(2013)	EN 60079-0	(2012)	A11:2013
EN 61326-2-3	(2013)	EN 60079-11	(2012)	
		EN 60079-26	(2007)	+Corrigendum 1

Certification EG-Baumusterprüfbescheinigung Nr. BVS 12 ATEX E 048 X
EC-Type Examination Certificate No.
Numéro de l'attestation d'examen CE de type
Ausgestellt von/issued by/délivré par DEKRA EXAM GmbH (0158)
Qualitätssicherung/Quality assurance/Système d'assurance DEKRA EXAM GmbH (0158)
qualité

Gerlingen, 20.04.2016
Endress+Hauser Conducta GmbH+Co. KG


i. V. Jörg-Martin Müller
Technology


i. V. Sven-Matthias Scheibe
Technology Certifications and Approvals

CLS50-G***


EU-Konformitätserklärung
EU-Declaration of Conformity
Déclaration UE de Conformité

Endress+Hauser 
 People for Process Automation



Company	Endress+Hauser Conducta GmbH+Co. KG Dieselstraße 24, 70839 Gerlingen, Germany erklärt als Hersteller in alleiniger Verantwortung, dass das Produkt declares as manufacturer under sole responsibility, that the product déclare sous sa seule responsabilité en qualité de fabricant que le produit	
Product	Indumax CLS50-G***	
Regulations	den folgenden Europäischen Richtlinien entspricht: conforms to following European Directives: est conforme aux prescription des Directives Européennes suivantes : EMC 2014/30/EU (L96/79) ATEX 2014/34/EU (L96/309)	
Standards	angewandte harmonisierte Normen oder normative Dokumente: applied harmonized standards or normative documents: normes harmonisées ou documents normatifs appliqués : EN 61326-1 (2013) EN 60079-0 (2012) + A11 (2013) EN 61326-2-3 (2013) EN 60079-11 (2012)	
Certification	EG-Baumusterprüfbescheinigung Nr. EC-Type Examination Certificate No. Numéro de l'attestation d'examen CE de type Ausgestellt von/issued by/délivré par Qualitätssicherung/Quality assurance/Système d'assurance qualité	DMT 99 ATEX 075 X DEKRA EXAM GmbH (0158) DEKRA EXAM GmbH (0158)

Gerlingen, 02.08.2016
 Endress+Hauser Conducta GmbH+Co. KG


 i. V. Jörg-Martin Müller
 Technology


 i. V. Robert Blinder
 Technology Certifications and Approvals

EC_00438_01.16

CLS50D-BV****

EU-Konformitätserklärung
EU-Declaration of Conformity
Déclaration UE de Conformité

Endress+Hauser 
People for Process Automation



Company **Endress+Hauser Conducta GmbH+Co. KG**
Dieselstraße 24, 70839 Gerlingen, Germany
erklärt als Hersteller in alleiniger Verantwortung, dass das Produkt
declares as manufacturer under sole responsibility, that the product
déclare sous sa seule responsabilité en qualité de fabricant que le produit

Product **Indumax**
CLS50D-BV****

Regulations den folgenden Europäischen Richtlinien entspricht:
conforms to following European Directives:
est conforme aux prescription des Directives Européennes suivantes :

EMC 2014/30/EU (L96/79)
ATEX 2014/34/EU (L96/309)
RoHS 2011/65/EU (L174/88)

Standards angewandte harmonisierte Normen oder normative Dokumente:
applied harmonized standards or normative documents:
normes harmonisées ou documents normatifs appliqués :

EN 61326-1	(2013)	EN 60079-0	(2012)	A11:2013
EN 61326-2-3	(2013)	EN 60079-11	(2012)	
EN 50581	(2012)			

Certification EG-Baumusterprüfbescheinigung Nr. -
EC-Type Examination Certificate No.
Numéro de l'attestation d'examen CE de type
Ausgestellt von/issued by/délivré par -
Qualitätssicherung/Quality assurance/Système d'assurance DEKRA EXAM GmbH (0158)
qualité

Gerlingen, 22.07.2017
Endress+Hauser Conducta GmbH+Co. KG


I. V. Jörg-Martin Müller
Technology


I. V. Sven-Matthias Scheibe
Technology Certifications and Approvals

CLS50-V***

EU-Konformitätserklärung
EU-Declaration of Conformity
Déclaration UE de Conformité

Endress+Hauser 
People for Process Automation



Company	Endress+Hauser Conducta GmbH+Co. KG Dieselstraße 24, 70839 Gerlingen, Germany erklärt als Hersteller in alleiniger Verantwortung, dass das Produkt declares as manufacturer under sole responsibility, that the product déclare sous sa seule responsabilité en qualité de fabricant que le produit
---------	--

Product	Indumax CLS50-V***
---------	-----------------------

Regulations den folgenden Europäischen Richtlinien entspricht:
conforms to following European Directives:
est conforme aux prescription des Directives Européennes suivantes :

EMC	2014/30/EU (L96/79)
ATEX	2014/34/EU (L96/309)
RoHS	2011/65/EU (L174/88)

Standards	angewandte harmonisierte Normen oder normative Dokumente: applied harmonized standards or normative documents: normes harmonisées ou documents normatifs appliqués :
------------------	--

EN 61326-1	(2013)	EN 60079-0	(2012)
EN 61326-2-3	(2013)	EN 60079-11	(2012) + A11 (2013)
EN 50581	(2012)		

Marking  II 3G Ex ic IIC T4/T6 Gc

Gerlingen, 31.05.2017
Endress+Hauser Conducta GmbH+Co. KG

i. V. Jörg-Martin Müller
Technology

i. V. Robert Binder
Technology Certifications and Approvals

EC 00440 02.16

Table of contents

1	About this document	7	10.2	Performance characteristics	36
1.1	Warnings	7	10.3	Environment	36
1.2	Symbols used	7	10.4	Process	37
1.3	Symbols on the device	8	10.5	Mechanical construction	39
2	Basic safety instructions	9	Index		42
2.1	Requirements for personnel	9			
2.2	Designated use	9			
2.3	Workplace safety	9			
2.4	Operational safety	10			
2.5	Product safety	10			
3	Incoming acceptance and product identification	14			
3.1	Incoming acceptance	14			
3.2	Product identification	14			
3.3	Scope of delivery	17			
3.4	Certificates and approvals	18			
4	Installation	19			
4.1	Installation conditions	19			
4.2	Mounting the sensor	21			
4.3	Post-installation check	24			
5	Electrical connection	24			
5.1	Connection conditions	25			
5.2	Connecting the sensor	29			
5.3	Ensuring the degree of protection	30			
5.4	Post-connection check	30			
6	Commissioning	31			
7	Maintenance	31			
8	Repair	32			
8.1	Spare parts	32			
8.2	Return	33			
8.3	Disposal	33			
9	Accessories	33			
9.1	Measuring cable	34			
9.2	Assemblies	34			
9.3	Calibration solutions	35			
10	Technical data	35			
10.1	Input	35			

1 About this document

1.1 Warnings

Structure of information	Meaning
 DANGER Causes (/consequences) If necessary, Consequences of non-compliance (if applicable) ► Corrective action	This symbol alerts you to a dangerous situation. Failure to avoid the dangerous situation will result in a fatal or serious injury.
 WARNING Causes (/consequences) If necessary, Consequences of non-compliance (if applicable) ► Corrective action	This symbol alerts you to a dangerous situation. Failure to avoid the dangerous situation can result in a fatal or serious injury.
 CAUTION Causes (/consequences) If necessary, Consequences of non-compliance (if applicable) ► Corrective action	This symbol alerts you to a dangerous situation. Failure to avoid this situation can result in minor or more serious injuries.
 NOTICE Cause/situation If necessary, Consequences of non-compliance (if applicable) ► Action/note	This symbol alerts you to situations which may result in damage to property.

1.2 Symbols used

Symbol	Meaning
	Additional information, tips
	Permitted or recommended
	Not permitted or not recommended
	Reference to device documentation
	Reference to page
	Reference to graphic
	Result of a step

1.3 Symbols on the device

Symbol	Meaning
	Reference to device documentation

2 Basic safety instructions

2.1 Requirements for personnel

- Installation, commissioning, operation and maintenance of the measuring system may be carried out only by specially trained technical personnel.
- The technical personnel must be authorized by the plant operator to carry out the specified activities.
- The electrical connection may be performed only by an electrical technician.
- The technical personnel must have read and understood these Operating Instructions and must follow the instructions contained therein.
- Faults at the measuring point may only be rectified by authorized and specially trained personnel.

 Repairs not described in the Operating Instructions provided must be carried out only directly at the manufacturer's site or by the service organization.

2.2 Designated use

Indumax CLS50D or CLS50 sensor is particularly suitable for use in the chemical and process technology sectors. The six-decade measuring range and the excellent chemical resistance properties of the materials in contact with the medium (PFA or PEEK) make it possible to use this sensor in a wide range of applications, such as:

- Concentration measurement of acids and bases
- Quality monitoring of chemical products in tanks and pipes
- Phase separation of product/product mixtures

The digital sensor CLS50D is used in conjunction with the Liquiline CM44x/R or Liquiline M CM42, while the analog sensor CLS50 is used with the Liquiline M CM42 or Liquisys CLM223/253.

Use of the device for any purpose other than that described, poses a threat to the safety of people and of the entire measuring system and is therefore not permitted.

The manufacturer is not liable for damage caused by improper or non-designated use.

2.3 Workplace safety

As the user, you are responsible for complying with the following safety conditions:

- Installation guidelines
- Local standards and regulations
- Regulations for explosion protection

Electromagnetic compatibility

- The product has been tested for electromagnetic compatibility in accordance with the applicable international standards for industrial applications.
- The electromagnetic compatibility indicated applies only to a product that has been connected in accordance with these Operating Instructions.

2.4 Operational safety

Before commissioning the entire measuring point:

1. Verify that all connections are correct.
2. Ensure that electrical cables and hose connections are undamaged.
3. Do not operate damaged products, and protect them against unintentional operation.
4. Label damaged products as defective.

During operation:

- If faults cannot be rectified:
products must be taken out of service and protected against unintentional operation.

2.5 Product safety

2.5.1 State-of-the-art technology

The product is designed to meet state-of-the-art safety requirements, has been tested, and left the factory in a condition in which it is safe to operate. The relevant regulations and international standards have been observed.

2.5.2 Electrical equipment in hazardous areas

Sensors with ATEX approval (CLS50-G*** and CLS50D-BA**** for Zone 0, CLS50-V*** and CLS50D-BV**** for Zone 2) have been developed and manufactured in compliance with applicable European standards and guidelines and are suitable for use in hazardous areas. The Declaration of Conformity confirms compliance with the harmonized European standards for using the sensors in hazardous areas.

CLS50D-BA**, CLS50D-IA****, CLS50D-GB****, CLS50D-NA****, CLS50D-H****, CLS50-G*** and CLS50-K*****

- The sensors may be operated in an environment specified as Ex Zone 0 (1G).
- The sensors may only be used in liquid media with a conductivity >10 nS/cm.
- If the connecting cable runs through Ex Zone 0 (1G), it must be protected against electrostatic charge.

CLS50D-BA**, CLS50D-IA****, CLS50D-NA**** and CLS50D-GB******

- The sensor is a digital sensor with the Memosens protocol and its connection values are those specified below.
- The sensor may also be connected to the intrinsically safe Memosens connection of the FSDG1 module of the Liquiline transmitter, types CM42-LE, CM42-LF, CM42-LI, EC type-examination certificate EX5 05 03 30266 012 (ATEX or IECEx) or CM42-LK (EAC Ex).
- The maximum permitted length of the measuring cable is 100 m (330 ft) here.

*Connection values of the CLS50D-BA****, CLS50D-IA**** and CLS50D-GB**** sensor*

U _i	5.1 V
I _i	130 mA
P _i	166 mW

C _i	18 µF
L _i	72 µH

*Temperature classes of CLS50D-BA****, CLS50D-IA**** and CLS50D-GB*****

Temperature class	Sensor	Ambient temperature range T _a	Medium temperature range T _{med}
T4	CLS50D-BA/IA/ GB*D** CLS50D-BA/IA/ GB*C** CLS50D-BA/IA/ GB*B**	-20 to +60 °C -20 to +60 °C -20 to +60 °C	-20 to +110 °C -20 to +120 °C -20 to +120 °C
T6	CLS50D-BA/IA/ GB*D** CLS50D-BA/IA/ GB*C** CLS50D-BA/IA/ GB*B**	-20 to +60 °C -20 to +60 °C -20 to +60 °C	-20 to +70 °C -20 to +70 °C -20 to +70 °C

CLS50-G***

- The sensor may only be connected to the following transmitters:
 - Liquiline types CM42-IG, CM42-IE, CM42-IF, EC type-examination certificate TÜV 13 ATEX 7459 X
 - Mycom type CLM153-Z with transmitter module type FCL1, EC type-examination certificate DMT 99 ATEX E 076
 - Mycom type CLM153-G, EC type-examination certificate DMT 01 ATEX E 174
- The maximum permitted length of the measuring cable is 55 m (180 ft) here.

*Temperature classes of CLS50-G****

Temperature class	Sensor	Ambient temperature range T _a	Medium temperature range T _{med}
T4	CLS50-G***	-20 to +125 °C	-20 to +125 °C
T6	CLS50-G***	-20 to +75 °C	-20 to +75 °C

CLS50D-BV**** and CLS50-V***

- The sensor may be operated in an environment specified as Ex Zone 2 (3G).
- The sensor may only be connected to the following transmitter:
 - Liquiline type CM42-LV (CLS50D) or CM42-IV (CLS50), EU Declaration of Conformity EC_00143_01.16
- Only CLS50-V***: The maximum permitted length of the measuring cable is 55 m (180 ft) here.

*Temperature classes of CLS50D-BV*****

Temperature class	Sensor	Ambient temperature range T _a	Medium temperature range T _{med}
T4	CLS50D-BV*D** CLS50D-BV*C** CLS50D-BV*B**	-20 to +60 °C -20 to +60 °C -20 to +60 °C	-20 to +110 °C -20 to +120 °C -20 to +120 °C
T6	CLS50D-BV****	-20 to +60 °C	-20 to +70 °C

*Temperature classes of CLS50-V****

Temperature class	Sensor	Ambient temperature range T _a	Medium temperature range T _{med}
T4	CLS50-V***	-20 to +125 °C	-20 to +125 °C
T6	CLS50-V***	-20 to +75 °C	-20 to +75 °C

CLS50-K***

- The sensor may only be connected to the following transmitter:
Liquiline type CM42-IK
- The maximum permitted length of the measuring cable is 55 m (180 ft) here.

*Temperature classes of CLS50-K****

Temperature class	Sensor	Ambient temperature range T _a	Medium temperature range T _{med}
T4	CLS50-K***	-20 to +125 °C	-20 to +125 °C
T6	CLS50-K***	-20 to +75 °C	-20 to +75 °C

Sensors with FM and CSA approval (CLS50D-FB**, CLS50D-C2****, CLS50-O***, CLS50-S****)**

Observe the documentation and the control drawings of the transmitter.

Sensors with NEPSI approval (CLS50D-NA** and CLS50-H*** for Zone 0, CLS50-V*** for Zone 2)**

Pay attention to the information on the NEPSI certificates. You can download these certificates from the product page: www.endress.com/cls50d or www.endress.com/cls50.

*Temperature classes of CLS50D-NA*****

Temperature class	Sensor	Ambient temperature range T _a	Medium temperature range T _{med}
T4	CLS50D-NA*D** CLS50D-NA*C** CLS50D-NA*B**	-20 to +60 °C -20 to +60 °C -20 to +60 °C	-20 to +110 °C -20 to +120 °C -20 to +120 °C
T6	CLS50D-NA*D** CLS50D-NA*C** CLS50D-NA*B**	-20 to +60 °C -20 to +60 °C -20 to +60 °C	-20 to +70 °C -20 to +70 °C -20 to +70 °C

*Temperature classes of CLS50-H****

Temperature class	Sensor	Ambient temperature range T _a	Medium temperature range T _{med}
T4	CLS50-H***	-20 to +125 °C	-20 to +125 °C
T6	CLS50-H***	-20 to +75 °C	-20 to +75 °C

Sensors with TIIS approval (CLS50D-TA**, CLS50-T****)**

Sensors with TIIS approval may only be used in a Zone 1 (2G) environment.

The following also applies for all the sensors listed

- Compliance with the specified ambient and medium temperature ranges is a prerequisite for safe use.
- The sensor must be connected and operated in accordance with the Operating Instructions of the sensor and of the transmitter to be connected. All sensor operating data must be observed.
- Avoid electrostatic charge. Metal process connections must be electrostatically connected ($R \leq 1 \text{ M}\Omega$).
- Non-metal process connections must be protected against electrostatic charge.
- In order to avoid electrostatic charge clean the sensor with a damp cloth only.
- Full compliance with regulations for electrical systems in hazardous locations (EN60079-14) is mandatory when using the devices and sensors.
- Ensure correct installation to maintain the housing protection type. (Use original seal. Fit cable entry properly. Tighten nut).
- The degree of protection only applies when the flange is mounted.

**CLS50 only**

In the CLS50 sensor, the internal sensor circuits are connected with the shielded wire of the supply cable. When installing the CM42 or CLM153 transmitter, the shielding of the sensor cable must be connected to functional ground as prescribed. As a result, the intrinsically safe sensor circuits of CLS50 are also connected to ground. Therefore, the power supply of the transmitter must be galvanically isolated and connected to ground. The CM42 and CLM153 transmitters already have secure internal galvanic isolation and therefore safely separate the sensor circuit from the other circuits.

3 Incoming acceptance and product identification

3.1 Incoming acceptance

1. Verify that the packaging is undamaged.

↳ Notify the supplier of any damage to the packaging.
Keep the damaged packaging until the issue has been resolved.
2. Verify that the contents are undamaged.

↳ Notify the supplier of any damage to the delivery contents.
Keep the damaged goods until the issue has been resolved.
3. Check that the delivery is complete and nothing is missing.

↳ Compare the shipping documents with your order.
4. Pack the product for storage and transportation in such a way that it is protected against impact and moisture.

↳ The original packaging offers the best protection.
Make sure to comply with the permitted ambient conditions.

If you have any questions, please contact your supplier or your local Sales Center.

3.2 Product identification

3.2.1 Type code for versions with explosion protection

Name	Type	Version									
Indumax		-	BA	x	x	x	x	+	x	x	
			For use in hazardous areas, ATEX II 1G Ex ia IIC T4/T6 Ga	Process connections, materials, cable connection, calibration, service No Ex relevance							

Name	Type	Version									
Indumax	CLS50D	-	IA	x	x	x	x	+	x	x	
			For use in hazardous areas, IECEx Ex ia IIC T4/T6 Ga	Process connections, materials, cable connection, calibration, service No Ex relevance							

Name	Type	Version									
Indumax	CLS50D	-	BV	x	x	x	x	+	x	x	
			For use in hazardous areas, ATEX II 3G Ex ic IIC T4/T6 Gc	Process connections, materials, cable connection, calibration, service No Ex relevance							

Name	Type	Version									
Indumax	CLS50D	-	NA	x	x	x	x	+	x	x	
			For use in hazardous areas, NEPSI Ex ia IIC T4/T6 Ga	Process connections, materials, cable connection, calibration, service No Ex relevance							

Name	Type	Version									
Indumax	CLS50D	-	C2	x	x	x	x	+	x	x	
			For use in hazardous areas, CSA IS NI C1.I Div.1&2, Gr. A-D	Process connections, materials, cable connection, calibration, service No Ex relevance							

Name	Type	Version									
Indumax	CLS50D	-	FB	x	x	x	x	+	x	x	
			For use in hazardous areas, FM IS NI C1.I Div.1&2, Gr. A-D	Process connections, materials, cable connection, calibration, service No Ex relevance							

Name	Type	Version									
Indumax	CLS50D	-	GB	x	B/C /D	x	x	+	x	x	
			For use in hazardous areas, EAC Ex, OEx ia IIC T6/T4 Ga X	Process connections, materials, cable connection, calibration, service No Ex relevance							

Name	Type	Version									
Indumax	CLS50D	-	TA	x	x	x	x	+	x	x	
			For use in hazardous areas, TIIS Ex ib IIC T4 Gb	Process connections, materials, cable connection, calibration, service No Ex relevance							

Name	Type	Version									
Indumax	CLS50	-	G	x	x	x					
			For use in hazardous areas, ATEX II 1G Ex ia IIC T4/T6 Ga	Process connections, materials, cable connection, calibration, service No Ex relevance							

Name	Type	Version					
Indumax	CLS50	-	V	x	x	x	
			For use in hazardous areas, ATEX II 3G Ex ic IIC T4/T6 Gc / NEPSI Ex ic IIC T4/T6 Gc	Process connections, materials, cable connection, calibration, service No Ex relevance			

Name	Type	Version					
Indumax	CLS50	-	H	x	x	x	
			For use in hazardous areas, NEPSI Ex ia IIC T4/T6 Ga	Process connections, materials, cable connection, calibration, service No Ex relevance			

Name	Type	Version					
Indumax	CLS50	-	O	x	x	x	
			For use in hazardous areas, FM IS NI Cl.I Div.1&2,Gr. A-D	Process connections, materials, cable connection, calibration, service No Ex relevance			

Name	Type	Version					
Indumax	CLS50	-	S	x	x	x	
			For use in hazardous areas, CSA IS NI Cl.I Div.1&2,Gr. A-D	Process connections, materials, cable connection, calibration, service No Ex relevance			

Name	Type	Version					
Indumax	CLS50	-	T	x	x	x	
			For use in hazardous areas, TIIS Ex ib IIC T4 Gb	Process connections, materials, cable connection, calibration, service No Ex relevance			

Name	Type	Version					
Indumax	CLS50	-	K	x	x	1/2 /3/ 4	
			For use in hazardous areas, EAC Ex, OEx ia IIC T6/T4 Ga X	Process connections, materials, cable connection, calibration, service No Ex relevance			

3.2.2 Nameplate

The nameplate provides you with the following information on your device:

- Manufacturer identification
- Order code
- Serial number
- Ambient and process conditions
- Safety information and warnings
- Cell constant (nominal value)
- Degree of protection
- Ex labeling on hazardous area versions

- ▶ Compare the information on the nameplate with the order.

3.2.3 Product identification

Product page

www.endress.com/cls50d

www.endress.com/cls50

Interpreting the order code

The order code and serial number of your product can be found in the following locations:

- On the nameplate
- In the delivery papers

Obtaining information on the product

1. Go to www.endress.com.
2. Call up the site search (magnifying glass).
3. Enter a valid serial number.
4. Search.
 - ↳ The product structure is displayed in a popup window.
5. Click on the product image in the popup window.
 - ↳ A new window (**Device Viewer**) opens. All of the information relating to your device is displayed in this window as well as the product documentation.

Manufacturer's address

Endress+Hauser Conducta GmbH+Co. KG
Dieselstraße 24
D-70839 Gerlingen

3.3 Scope of delivery

The scope of delivery includes:

- Sensor in the version ordered
- Operating Instructions

- If you have any queries:
Please contact your supplier or local sales center.

3.4 Certificates and approvals

3.4.1 CE mark

Declaration of Conformity

The product meets the requirements of the harmonized European standards. As such, it complies with the legal specifications of the EU directives. The manufacturer confirms successful testing of the product by affixing to it the **CE** mark.

3.4.2 Ex approvals

CLS50D-BA** and CLS50-G******

ATEX II 1G Ex ia IIC T4/T6 Ga

CLS50D-BV****

ATEX II 3G Ex ic IIC T4/T6 Gc

CLS50D-IA****

IECEX Ex ia IIC T4/T6 Ga

CLS50-V****

ATEX II 3G Ex ic IIC T4/T6 Gc + NEPSI Ex ic IIC T4/T6 Gc

CLS50D-NA** and CLS50-H******

NEPSI Ex ia IIC T4/T6 Ga

CLS50D-FB** and CLS50-O******

FM IS NI Cl.I Div.1&2,G. A-D

CLS50D-C2** and CLS50-S******

CSA IS NI Cl.I Div.1&2,Gr. A-D

CLS50D-TA** and CLS50-T******

TIIS Ex ib IIC T4 Gb

CLS50D-GB** and CLS50-K******

- EAC Ex, OEx ia IIC T6/T4 Ga X
- Zone 0
- Certificate number: TC RU C-DE.AA87.B.00088 and TC RU C-DE.ГБ05.B.00172 (only CLS50-K****)
- The product has been certified in accordance with Directive TR CU 012/2011 which applies in the European Economic Area (EEA). The EAC conformity mark has been affixed to the product.

3.4.3 Certification body (only CLS50D-GB and CLS50-K)

ООО "НАИЮ ЦСБЭ"

Russian Federation

3.4.4 Marine approvals


A selection of sensors have type approval for marine applications, issued by the following classification societies: ABS (American Bureau of Shipping), BV (Bureau Veritas), DNV-GL (Det Norske Veritas-Germanische Lloyd) and LR (Lloyd's Register). Details of the order codes of the approved sensors, and the installation and ambient conditions, are provided in the relevant certificates for marine applications on the product page on the Internet.

4 Installation

4.1 Installation conditions

4.1.1 Installation position

- When installing, align the sensor in such a way that the medium flows through the flow opening of the sensor in the direction of medium flow.
 - ↳ The sensor head must be completely immersed in the medium.

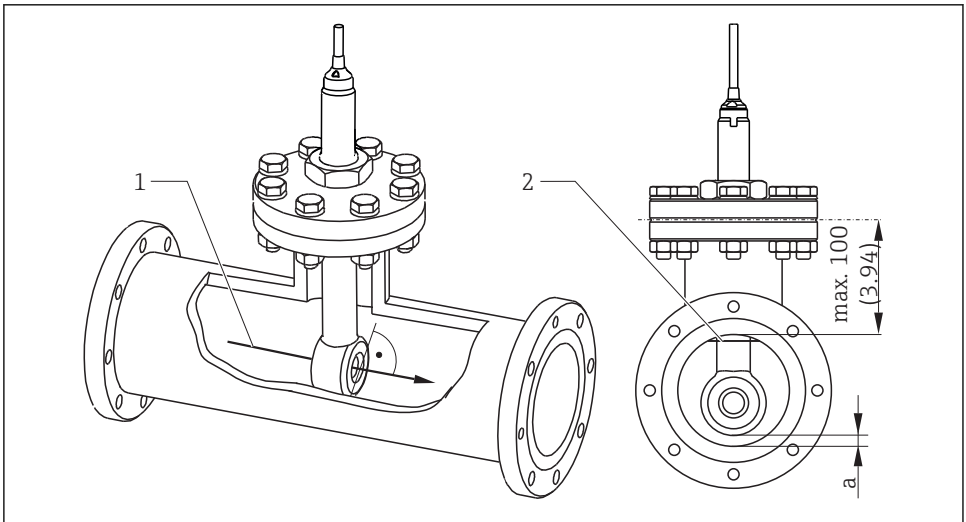

A0036463


1 Sensor orientation, dimensions in mm (in)

- 1 Direction of medium flow
- 2 Minimum water level in the pipe
- a Distance from pipe wall

4.1.2 Installation factor

In confined installation conditions, the conductivity measurement is affected by the pipe walls. The installation factor compensates for this effect. The transmitter corrects the cell constant

by multiplying by the installation factor. The value of the installation factor depends on the diameter and the conductivity of the pipe nozzle as well as the sensor's distance to the wall. The installation factor f can be disregarded ($f = 1.00$) if the distance to the wall is sufficient ($a > 15 \text{ mm}$ (0.59"), from DN 80). If the distance to the wall is smaller, the installation factor increases for electrically insulating pipes ($f > 1$) and decreases for electrically conductive pipes ($f < 1$). It can be measured using calibration solutions, or a close approximation determined from the following diagram.

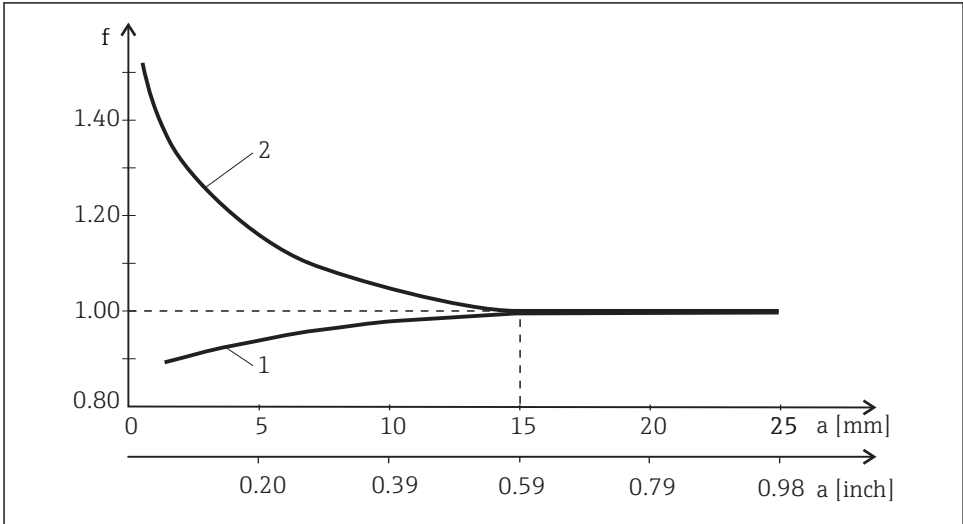

A0034874

2 Relationship between installation factor f and wall distance

- 1 Electrically conductive pipe wall
- 2 Electrically insulating pipe wall

4.1.3 Air set

CLS50D

The digital sensor has already been adjusted at the factory. Onsite compensation is not required.

CLS50

To compensate residual coupling in the cable and between the two sensor coils, zero adjustment in air ("air set") must be performed before installing the sensor. Follow the instructions provided in the Operating Instructions of the transmitter used.

4.2 Mounting the sensor

4.2.1 Installation with flange

The sensor is suitable for installation in T-pieces $\geq$ DN 80, with the outgoing diameter reduced to $\geq$ DN 50.


WARNING

Leakage

Risk of injury if medium escapes!

- ▶ Tighten sensor nut using a torque of 20 Nm.
- ▶ To avoid leakages, regularly check the tightness of the nut.

Flange, not in contact with medium

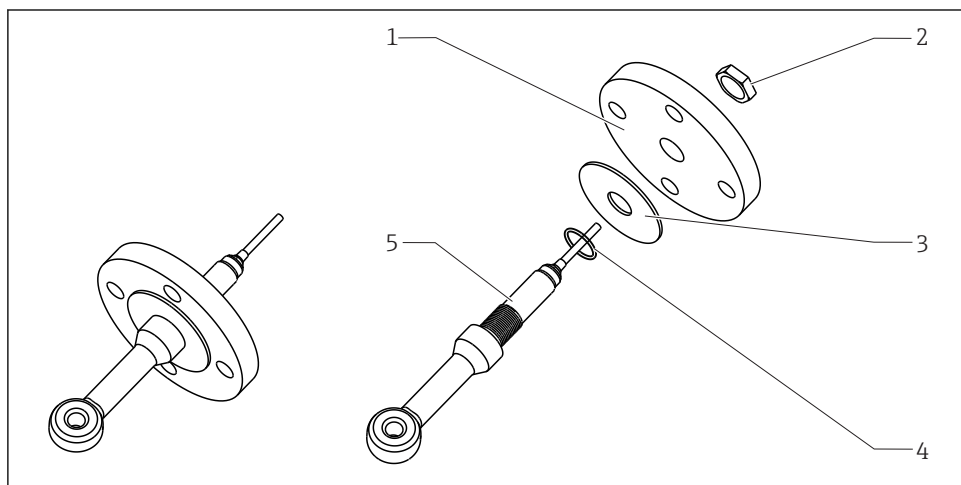


A0024949

 3 Fixed flange, not in contact with medium (for order option: "Process connection" = 5, 6, 7)

- 1 Flange (stainless steel)
- 2 Nut
- 3 Sealing disk (GYLON)
- 4 O-ring
- 5 Sensor


Flange, in contact with medium

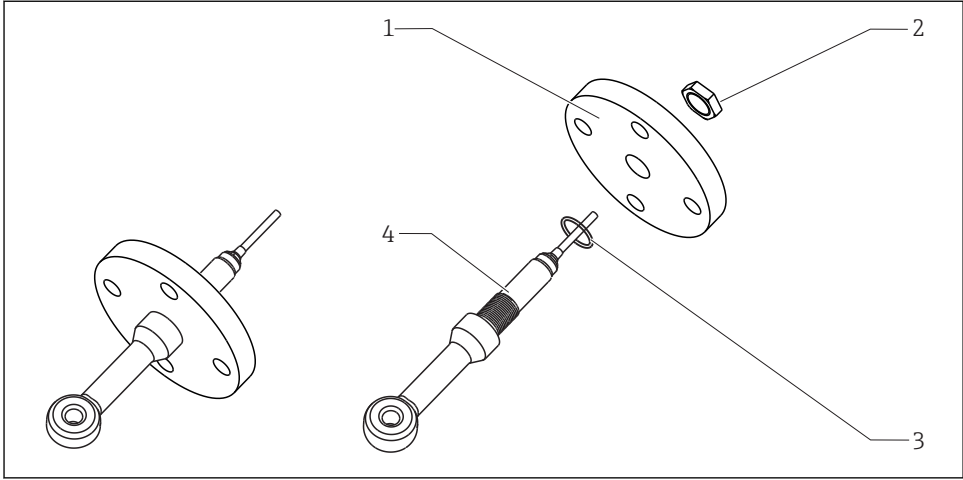

A0024953

■ 4 Fixed flange, in contact with medium (for order option: "Process connection" = 3, 4)

- 1 Flange (stainless steel)
- 2 Nut
- 3 O-ring
- 4 Sensor

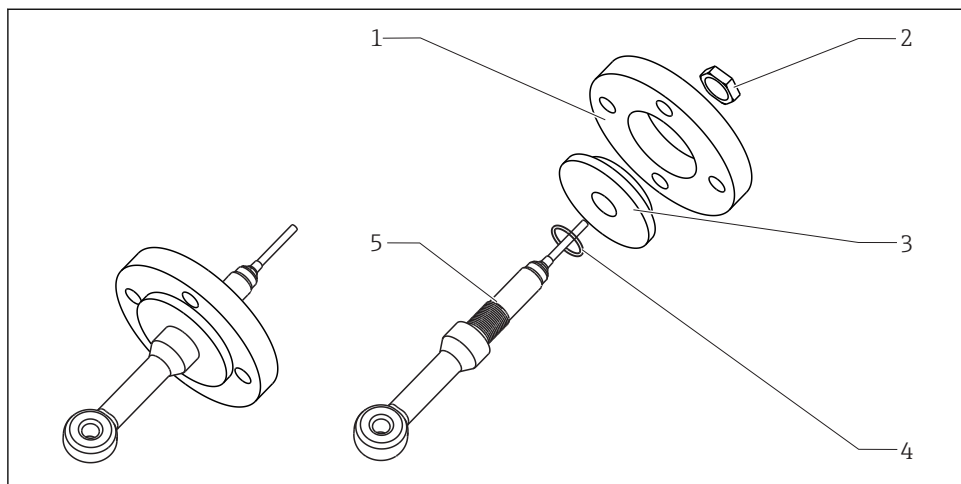Lap joint flange, not in contact with medium

A0024954

 5 *Lap joint flange, not in contact with medium (for order option: "Process connection" = A, B, C)*

1 *Lap joint flange (PP-GF)*


2 *Nut (stainless steel)*

3 *Flange (PVDF)*

4 *O-ring*

5 *Sensor*

4.2.2 Installation in assembly

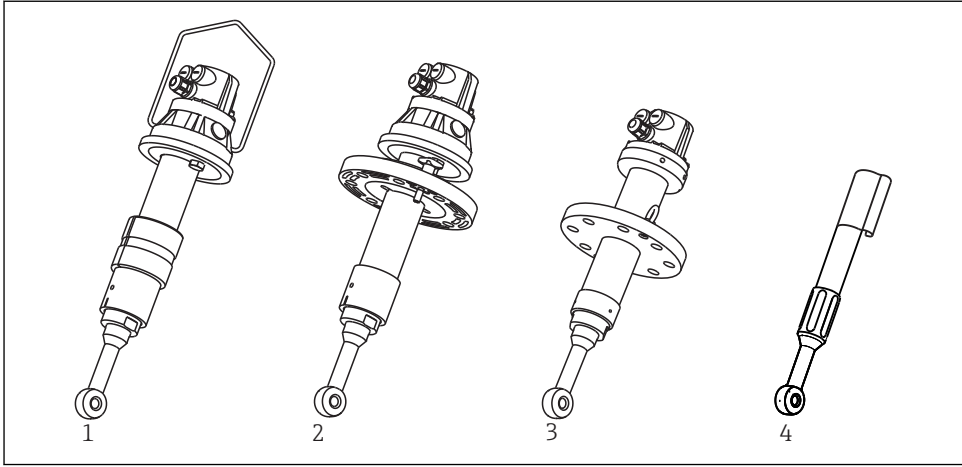

A0024960

 6 Installation of sensor with assembly

- 1 CLA111 with suspension bracket
- 2 CLA111 with flange connection
- 3 CLA140 with flange connection
- 4 CYA112

4.3 Post-installation check

Put the sensor into operation only if you can answer yes to the following questions:

1. Are the sensor and cable undamaged?
2. Is the orientation correct (arrow on threaded sleeve=flow direction=installation direction)?
3. Has the sensor been installed in the process connection, and does not suspend freely from the cable?

5 Electrical connection

WARNING


Device is live!

Incorrect connection may result in injury or death!

- The electrical connection may be performed only by an electrical technician.
- The electrical technician must have read and understood these Operating Instructions and must follow the instructions contained therein.
- **Prior** to commencing connection work, ensure that no voltage is present on any cable.


5.1 Connection conditions

5.1.1 Connection diagram: sensors for Zone 0 (ATEX/EAC Ex)

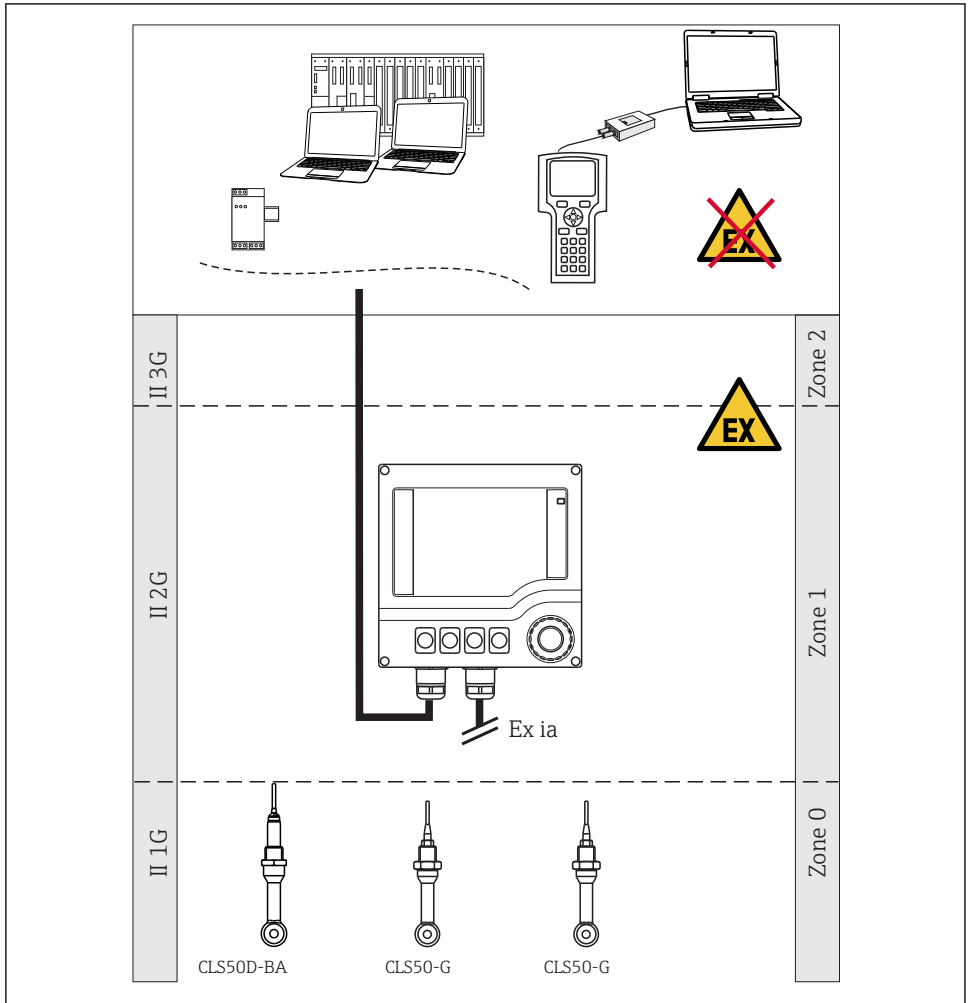


A0013258

5.1.2 Connection diagram: sensors for Zone 0 (IECEEx)

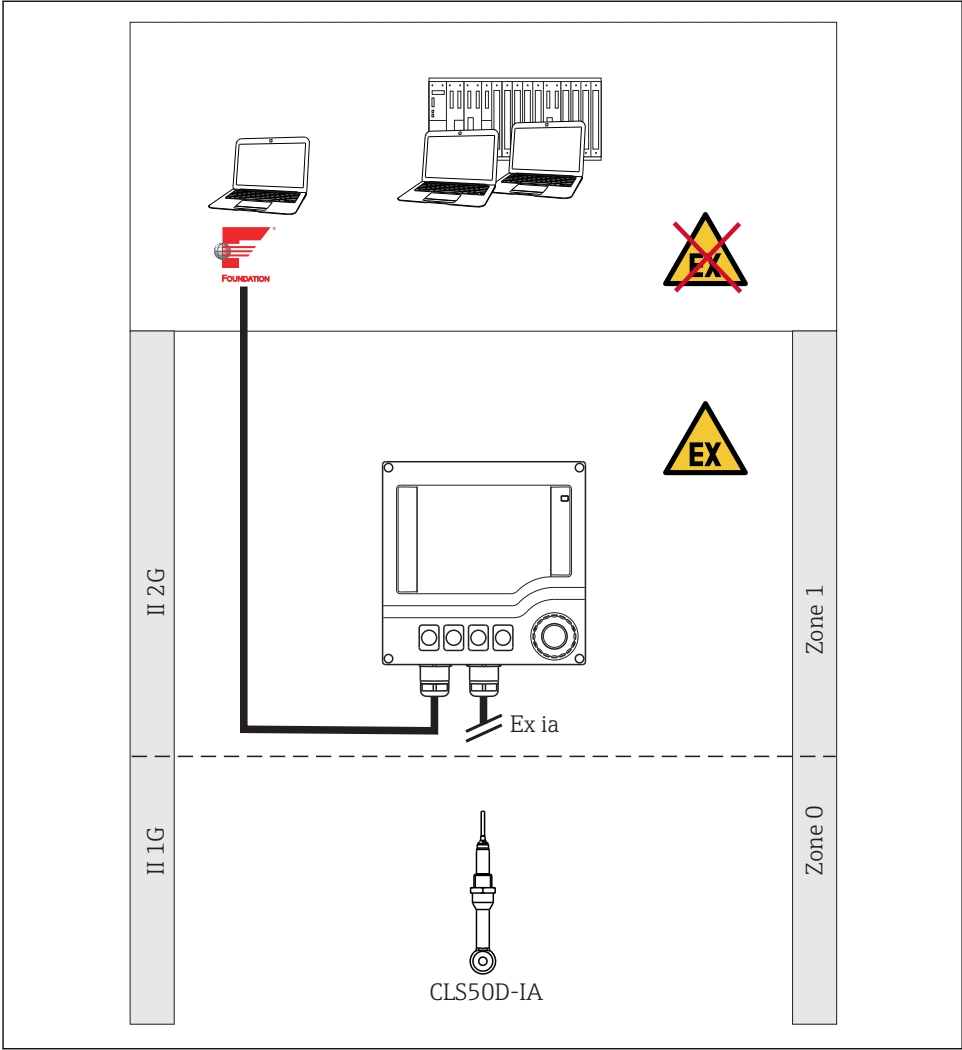


A0025482

5.1.3 Connection diagram: sensors for Zone 0 (NEPSI)

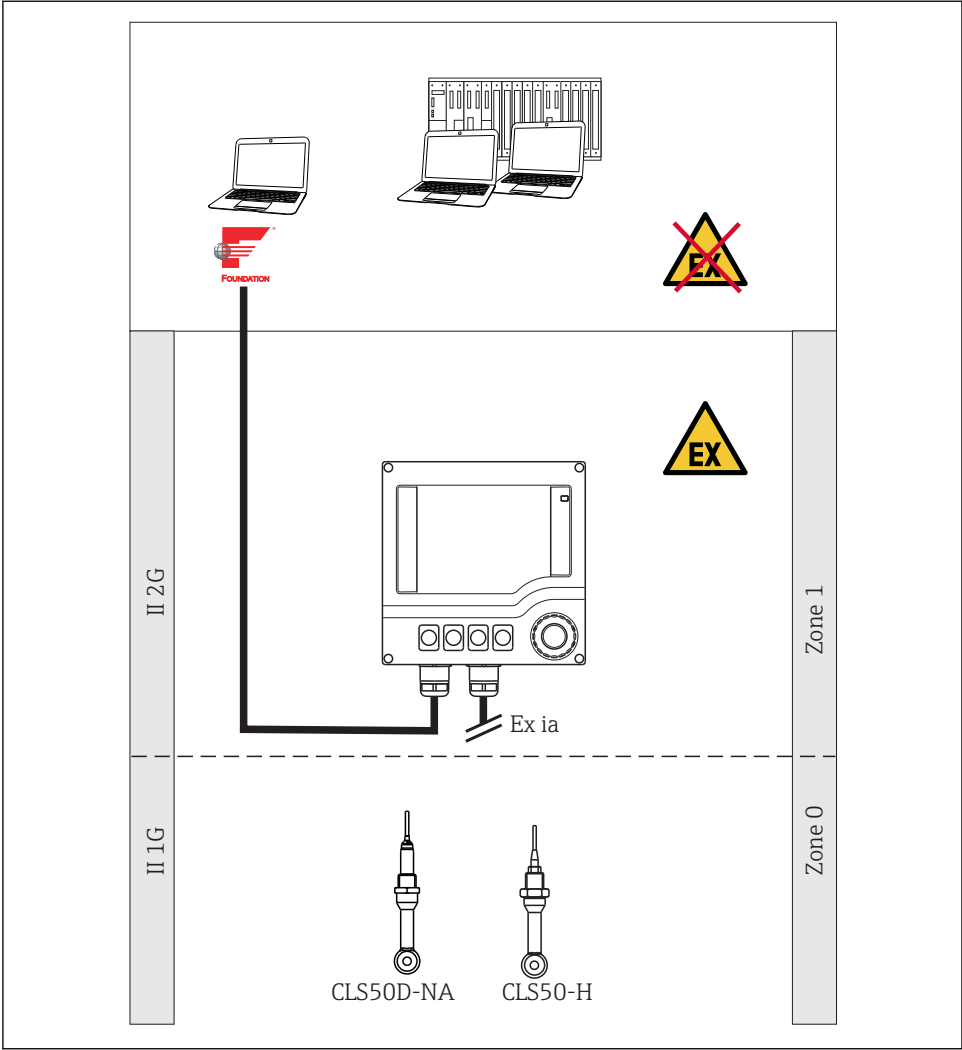

A0025481

5.1.4 Connection diagram: sensors for Zone 2 (ATEX/NEPSI)

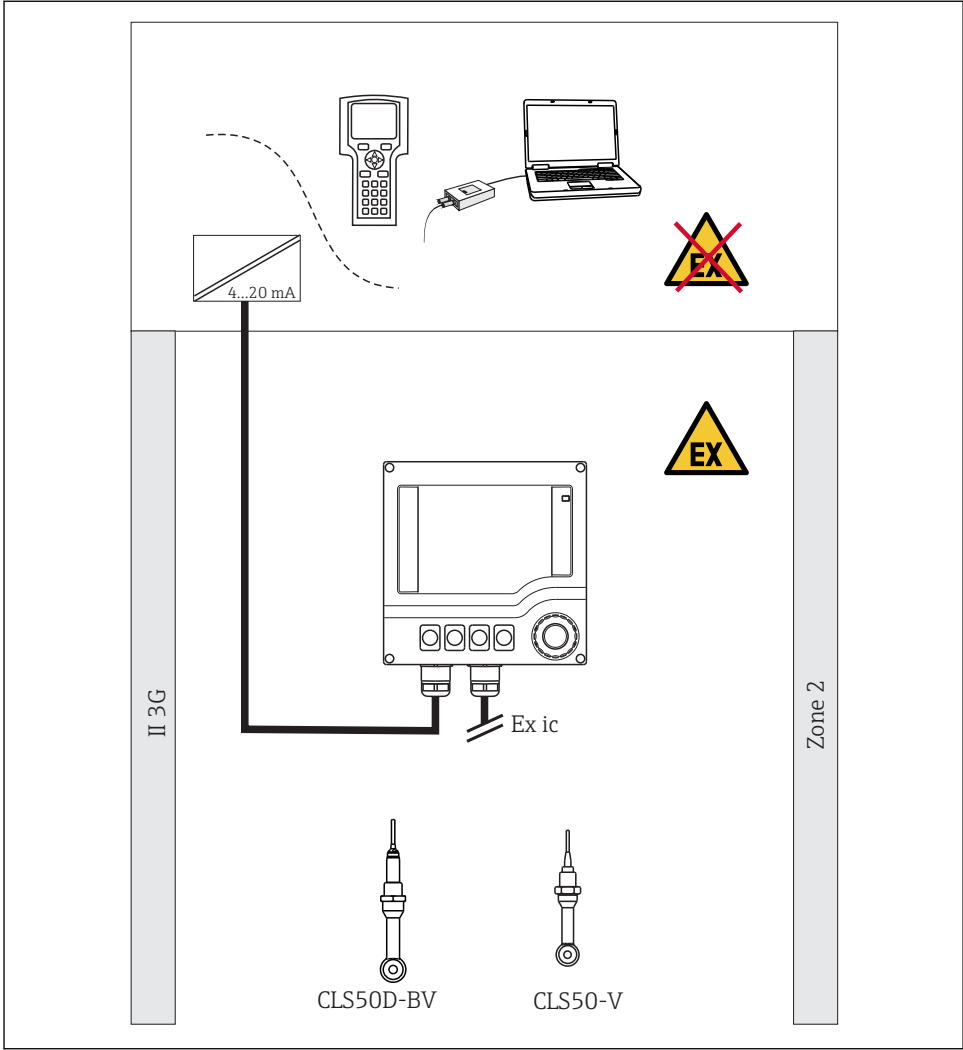


A0010316

5.1.5 Sensors with FM or CSA approval

The instructions in the Control Drawing apply for sensors with FM or CSA approval. You can find the Control Drawing in the Operating Instructions of the transmitter used.


5.2 Connecting the sensor

5.2.1 Direct connection, e.g. to CM42

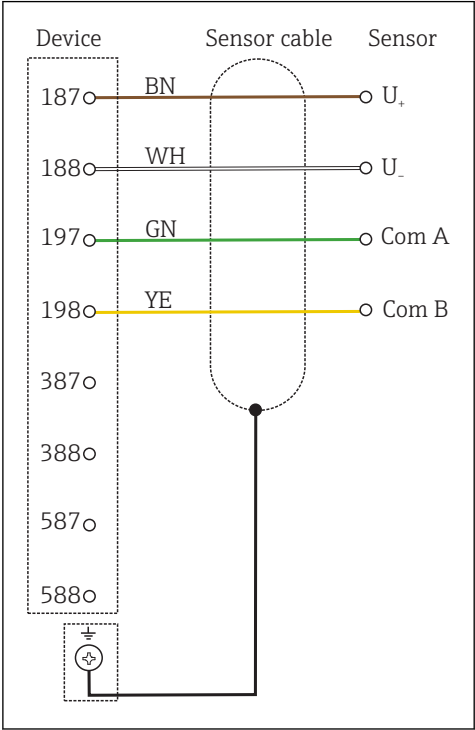

A0001078

7 CLS50D to CM42

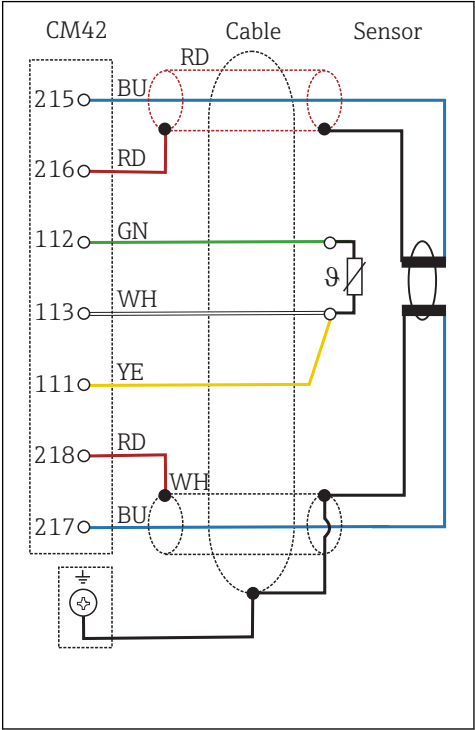


A0001082

8 CLS50 to CM42

5.2.2 Cable extension

The sensor is supplied with a fixed cable. The cable between the sensor and transmitter can be extended using the CYK11 (CLS50D) or CLK6 (CLS50) measuring cable (does not apply for use in a hazardous environment).

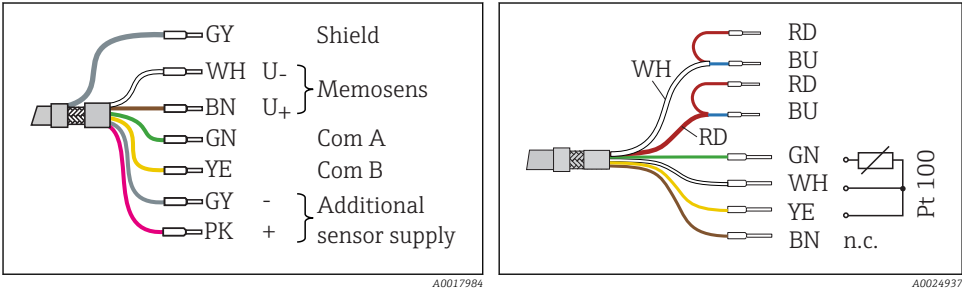

9 CYK11 for extension of CLS50D

10 CLK6 for extension of CLS50

Total cable length (max.): 100 m (330 ft)

Total cable length (max.): 55 m (180 ft)

i CLS50 only:
The residual coupling of the sensor increases when the fixed cable is extended.

5.3 Ensuring the degree of protection

Only the mechanical and electrical connections which are described in these instructions and which are necessary for the required, designated use, may be carried out on the device delivered.

► Exercise care when carrying out the work.

Otherwise, the individual types of protection (Ingress Protection (IP), electrical safety, EMC interference immunity) agreed for this product can no longer be guaranteed due, for example to covers being left off or cable (ends) that are loose or insufficiently secured.

5.4 Post-connection check

Device condition and specifications	Action
Are the sensor, assembly, or cables free from damage on the outside?	► Perform a visual inspection.
Electrical connection	Action
Are the mounted cables strain-relieved and not twisted?	► Untwist the cables.
Is a sufficient length of the cable cores stripped, and are the cores positioned in the terminal correctly?	► Pull gently to check they are seated correctly.
Are all the screw terminals properly tightened?	► Tighten the screw terminals.
Are all cable entries mounted, tightened and leak-tight?	In the case of lateral cable entries:
Are all cable entries installed downwards or mounted laterally?	► Point cable loops downward so that water can drip off.

6 Commissioning

Prior to initial commissioning, ensure that:

- The sensor is correctly installed
- The electrical connection is correct

If using an assembly with automatic cleaning function:

- ▶ Check that the cleaning medium (water or air, for example) is connected correctly.

WARNING

Escaping process medium

Risk of injury from high pressure, high temperatures or chemical hazards!

- ▶ Before applying pressure to an assembly with cleaning system, ensure that the system has been connected correctly.
 - ▶ If you cannot reliably establish the correct connection, do not install the assembly in the process.
 - ▶ At the transmitter, enter all the settings specific to the parameters and measuring point.
- The measuring point is then ready to measure.



Following commissioning, the sensor must be serviced at regular intervals, as only then can reliable measurement be guaranteed.



Operating Instructions for the transmitter used, such as BA01245C if using the Liquiline CM44x or CM44xR.

7 Maintenance

WARNING

Thiocarbamide

Harmful if swallowed! Limited evidence of carcinogenicity! Possible risk of harm to the unborn child! Dangerous for the environment with long-term effects!

- ▶ Wear protective goggles, protective gloves and appropriate protective clothing.
- ▶ Avoid all contact with the eyes, mouth and skin.
- ▶ Avoid discharge into the environment.

Clean away fouling on the sensor as follows depending on the type of fouling:

1. Oily and greasy films:

Clean with fat solvent, e.g. alcohol, or hot water and agents containing surfactants (alkaline) (e.g. dishwashing detergent).

2. Lime and metal hydroxide buildup and low solubility (lyophobic) organic buildup:


Dissolve buildup with diluted hydrochloric acid (3 %) and then rinse thoroughly with plenty of clear water.


3. Sulfidic buildup (from flue gas desulfurization or wastewater treatment plants):
Use a mixture of hydrochloric acid (3 %) and thiocarbamide (commercially available) and then rinse thoroughly with plenty of clear water.
4. Buildup containing proteins (e.g. food industry):
Use a mixture of hydrochloric acid (0.5 %) and pepsin (commercially available) and then rinse thoroughly with plenty of clear water.
5. Readily soluble biological buildup:
Rinse with pressurized water.

After cleaning, rinse the sensor thoroughly with water.

8 Repair

8.1 Spare parts

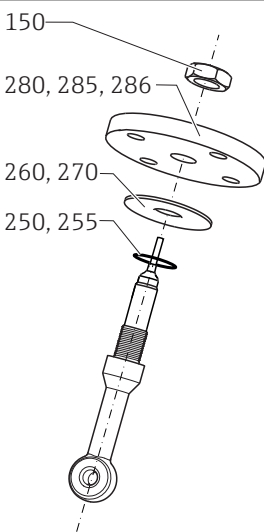	Item No.	Spare parts kit	Order No.
 A0025483	150, 255	CHEMRAZ seal kit ▪ Nut (item 150) ▪ CHEMRAZ O-ring, 2 pcs. (item 255)	71086368
	150, 250	VITON seal kit ▪ Nut (item 150) ▪ VITON O-ring, 3. pcs., (item 250)	71086369
	260	PTFE disk kit for DN 50	71086372
	270	PTFE disk kit for ANSI 2" and JIS 10K 50A	71086374
	150, 280	Fixed flange kit, DN 50, stainless steel 1.4404 (AISI 316L) ▪ Nut (item 150) ▪ Flange DN 50 (item 280)	51500525
	150, 285	Fixed flange kit, ANSI 2", stainless steel 1.4404 (AISI 316L) ▪ Nut (item 150) ▪ Flange ANSI 2" (item 285)	51500527
	150, 286	Fixed flange kit, JIS, stainless steel 1.4404 (AISI 316L) ▪ Nut (item 150) ▪ Flange DN 50 (item 286)	51500934

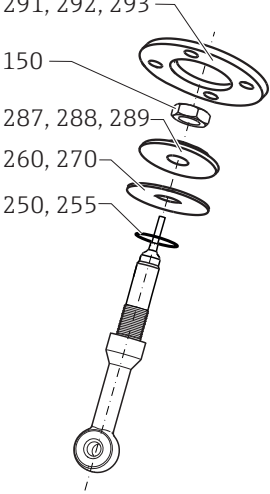	Item No.	Spare parts kit	Order No.
	150, 288, 292	Lap joint flange kit, ANSI 2", PVDF ■ Nut (item 150) ■ Flange ANSI 2", PVDF (item 288) ■ Lap joint flange, UP-GF (item 292)	51500937
	150, 287, 291	Lap joint flange kit, DN 50, PVDF ■ Nut (item 150) ■ Flange DN 50, PVDF (item 287) ■ Lap joint flange, UP-GF (item 291)	51500936
	150, 289, 293	Lap joint flange kit, JIS, PVDF ■ Nut (item 150) ■ Flange JIS, PVDF (item 289) ■ Lap joint flange, UP-GF (item 293)	51500935

8.2 Return

The product must be returned if repairs or a factory calibration are required, or if the wrong product was ordered or delivered. As an ISO-certified company and also due to legal regulations, Endress+Hauser is obliged to follow certain procedures when handling any returned products that have been in contact with medium.

To ensure the swift, safe and professional return of the device:

- Refer to the website www.endress.com/support/return-material for information on the procedure and conditions for returning devices.

8.3 Disposal

The device contains electronic components. The product must be disposed of as electronic waste.

- Observe the local regulations.

9 Accessories

The following are the most important accessories available at the time this documentation was issued.

- For accessories not listed here, please contact your Service or Sales Center.

9.1 Measuring cable

9.1.1 For CLS50D

Memosens data cable CYK11

- Extension cable for digital sensors with Memosens protocol
- Product Configurator on the product page: www.endress.com/cyk11



Technical Information TI00118C

9.1.2 For CLS50

Measuring cable CLK6

- Extension cable for inductive conductivity sensors, for extension via VBM junction box
- Sold by the meter, order number: 71183688

VBM

- Junction box for cable extension
- 10 terminal strips
- Cable entries: 2 x Pg 13.5 or 2 x NPT ½"
- Material: aluminum
- Degree of protection: IP 65
- Order numbers
 - Cable entries Pg 13.5 : 50003987
 - Cable entries NPT ½": 51500177

9.2 Assemblies

Dipfit CLA111

- Immersion assembly for open and closed vessels with flange DN 100
- Product Configurator on the product page: www.products.endress.com/cla111



Technical Information TI00135C

Dipfit CLA140

- For the CLS50/CLS50D inductive sensor
- Immersion assembly with flange connection for very demanding processes
- Product Configurator on the product page: www.products.endress.com/cla140



Technical Information TI00196C

Flexdip CYA112

- Immersion assembly for water and wastewater
- Modular assembly system for sensors in open basins, channels and tanks
- Material: PVC or stainless steel
- Product Configurator on the product page: www.endress.com/cya112



Technical Information TI00432C

9.3 Calibration solutions

Conductivity calibration solutions CLY11

Precision solutions referenced to SRM (Standard Reference Material) by NIST for qualified calibration of conductivity measuring systems in accordance with ISO 9000

- CLY11-B, 149.6 $\mu\text{S}/\text{cm}$ (reference temperature 25 °C (77 °F)), 500 ml (16.9 fl.oz)
Order No. 50081903
- CLY11-C, 1.406 mS/cm (reference temperature 25 °C (77 °F)), 500 ml (16.9 fl.oz)
Order No. 50081904
- CLY11-D, 12.64 mS/cm (reference temperature 25 °C (77 °F)), 500 ml (16.9 fl.oz)
Order No. 50081905
- CLY11-E, 107.00 mS/cm (reference temperature 25 °C (77 °F)), 500 ml (16.9 fl.oz)
Order No. 50081906



Technical Information TI00162C

10 Technical data

10.1 Input

10.1.1 Measured variables

- Conductivity
- Temperature

10.1.2 Measuring range

Conductivity	2 $\mu\text{S}/\text{cm}$ to 2000 mS/cm (uncompensated)
Temperature	-20 to +180 °C (-4 to +350 °F)

10.1.3 Cell constant

$k = 1.98 \text{ cm}^{-1}$

10.1.4 Measuring frequency

2 kHz

10.1.5 Temperature measurement

CLS50D

Pt1000 (Class A according to IEC 60751)

CLS50

Pt100 (Class A according to IEC 60751)

10.2 Performance characteristics

10.2.1 Conductivity response time

$t_{95} \leq 2 \text{ s}$

10.2.2 Temperature response time

PEEK version: $t_{90} \leq 7 \text{ min}$

PFA version: $t_{90} \leq 11 \text{ min}$

10.2.3 Maximum measured error

-20 to 100 °C (-4 to 212 °F): $\pm(5 \text{ }\mu\text{S/cm} + 0.5 \% \text{ of reading})$

> 100 °C (212 °F): $\pm(10 \text{ }\mu\text{S/cm} + 0.5 \% \text{ of reading})$

10.2.4 Repeatability

For $T < 100 \text{ }^{\circ}\text{C}$ (212 °F): 0.2 % of reading + 1 $\mu\text{S/cm}$

For $T > 100 \text{ }^{\circ}\text{C}$ (212 °F): 0.2 % of reading + 2 $\mu\text{S/cm}$

10.2.5 Linearity

1.9 % (only applies in the 1 to 20 mS/cm measuring range)

10.3 Environment

10.3.1 Ambient temperature

CLS50D

-10 to +60 °C (+10 to +140 °F)

CLS50

-10 to +70 °C (+10 to +160 °F)

10.3.2 Storage temperature

-20 to +80 °C (0 to +180 °F)

10.3.3 Degree of protection

IP 68 / NEMA type 6 (sensor in installed state with genuine seal)

10.4 Process

10.4.1 Process temperature

Sensor material	CLS50D-*1/2 Without flange	CLS50D-*3/4/5/6/8 DN50, ANSI 2"	CLS50D-*7 JIS	CLS50D-*A/B/C PVDF lap joint flange
PEEK	-20 to 125 °C (-4 to 260 °F)	-20 to 125 °C (-4 to 260 °F)	-20 to 125 °C (-4 to 260 °F)	-20 to 125 °C (-4 to 260 °F)
PFA	-20 to 110 °C (-4 to 230 °F)	-20 to 110 °C (-4 to 230 °F)	-20 to 110 °C (-4 to 230 °F)	-20 to 110 °C (-4 to 230 °F)

CLS50


Sensor material	CLS50-*1/2 Without flange	CLS50-*3/4/5/6/8 DN50, ANSI 2"	CLS50-*7 JIS	CLS50-*A/B/C PVDF lap joint flange
PEEK	-20 to 180 °C (-4 to 360 °F)	-20 to 180 °C (-4 to 360 °F)	-20 to 180 °C (-4 to 360 °F)	-20 to 125 °C (-4 to 260 °F)
PFA	-20 to 125 °C (-4 to 260 °F)	-20 to 125 °C (-4 to 260 °F)	-20 to 125 °C (-4 to 260 °F)	-20 to 125 °C (-4 to 260 °F)

10.4.2 Process pressure (absolute)

Max. 21 bar (305 psi), depending on the sensor version, see pressure-temperature ratings

10.4.3 Temperature/pressure ratings

CLS50D

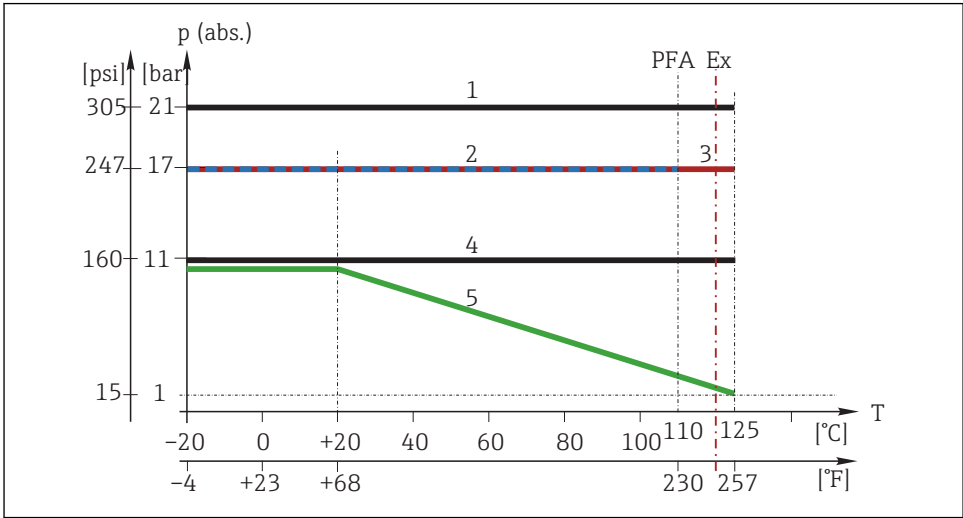


A0024981

11 Pressure temperature ratings CLS50D

- 1 PEEK sensor, without a flange
- 2 PFA sensor, without a flange (blue line)
- 3 PEEK or PFA sensor, with DN50/ANSI 2" flange (red line)
- 4 PEEK or PFA sensor, with JIS flange
- 5 PEEK or PFA sensor, with PVDF lap joint flange (green line)

CLS50

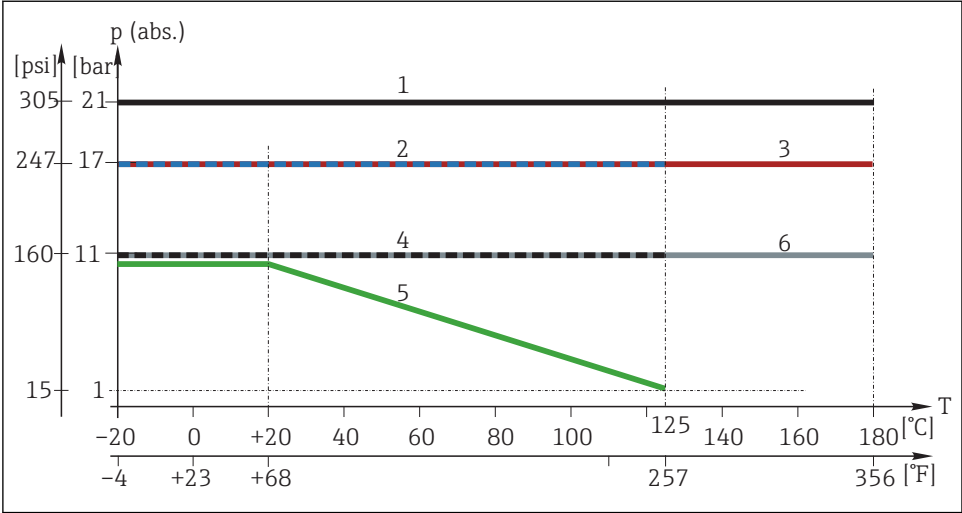

A0024979

12 Pressure-temperature ratings for CLS50

- 1 PEEK sensor, without a flange
- 2 PFA sensor, without a flange or with DN50/ANSI 2" flange (blue line)
- 3 PEEK sensor, with DN50/ANSI 2" flange (red line)
- 4 PFA sensor, with JIS flange (black line)
- 5 PEEK or PFA sensor, with PVDF lap joint flange (green line)
- 6 PEEK sensor, with JIS flange (gray line)

10.5 Mechanical construction

10.5.1 Weight

Approx. 0.65 kg (1.43 lbs)

10.5.2 Materials


Sensor	PEEK, PFA (depending on version)
Sensor seal	VITON, CHEMRAZ (depending on version)

Process connections	
G¾	CLS50D-*1B/C**: PEEK GF30 CLS50D-*1D**: stainless steel (AISI 316Ti) CLS50-*1A*: stainless steel 1.4571 (AISI 316Ti) CLS50-*1B/C/1/2/3: PEEK GF30 CLS50-*1B/C5/6: stainless steel 1.4571 (AISI 316Ti)
NPT 1"	PEEK
Fixed flange	Stainless steel 1.4404 (AISI 316L)
Sealing disk	GYLON (PTFE ceramic-filled)
Lap joint flange	PP-GF
Flange combined with lap joint flange	PVDF

10.5.3 Process connections

- G¾ thread
- NPT 1" thread
- Lap joint flange EN 1092 DN50 PN10
- Lap joint flange ANSI 2" 150 lbs
- Lap joint flange JIS 10K 50A
- Flange EN 1092-1 DN50 PN16
- Flange ANSI 2" 300 lbs
- Flange JIS 10K 50A

Flange dimensions

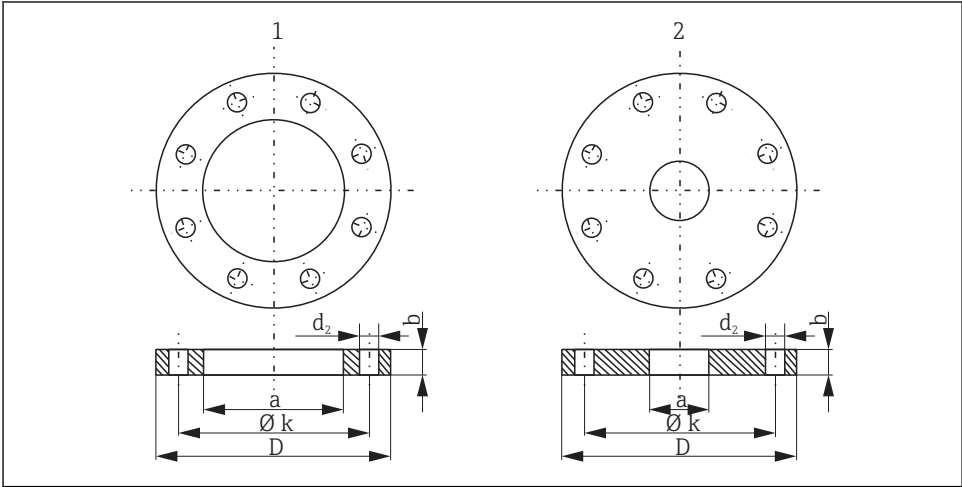

A0024986

13 Flange dimensions

- 1 Lap joint flange (PP-GF)
2 Fixed flange (stainless steel)

Dimensions in mm

Lap joint flange PP-GF	DN50 PN10	ANSI 2" 150 lbs	JIS 10K 50A
D	165	165	152
Ø k	125	121	120
d₂	4 x 18	8 x 19	4 x 19
b	18	18	18
a	78	78	78
Screws	M16	M16	M16

Dimensions in mm

Fixed flange SS 316 L	DN50 PN10	ANSI 2" 300 lbs	JIS 10K 50A
D	165	165.1	155
Ø k	125	127	120
d₂	4 x 18	8 x 19	4 x 19
b	18	22.2	16
a	27	27	27
Screws	M16	M16	M16

10.5.4 Chemical resistance

Medium	Concentration	PEEK	PFA	CHEMRAZ	VITON
Sodium hydroxide solution NaOH	0 to 50 %	20 to 100 °C (68 to 212 °F)	20 to 50 °C (68 to 122 °F)	0 to 150 °C (32 to 302 °F)	Not suitable
Nitric acid HNO ₃	0 to 10 %	20 to 100 °C (68 to 212 °F)	20 to 80 °C (68 to 176 °F)	0 to 150 °C (32 to 302 °F)	0 to 120 °C (32 to 248 °F)
	0 to 40 %	20 °C (68 °F)	20 to 60 °C (68 to 140 °F)	0 to 150 °C (32 to 302 °F)	0 to 120 °C (32 to 248 °F)
Phosphoric acid H ₃ PO ₄	0 to 80 %	20 to 100 °C (68 to 212 °F)	20 to 60 °C (68 to 140 °F)	0 to 150 °C (32 to 302 °F)	0 to 120 °C (32 to 248 °F)
Sulfuric acid H ₂ SO ₄	0 to 2.5 %	20 to 80 °C (68 to 176 °F)	20 to 100 °C (68 to 212 °F)	0 to 150 °C (32 to 302 °F)	0 to 120 °C (32 to 248 °F)
	0 to 30 %	20 °C (68 °F)	20 to 100 °C (68 to 212 °F)	0 to 150 °C (32 to 302 °F)	0 to 120 °C (32 to 248 °F)
Hydrochloric acid HCl	0 to 5 %	20 to 100 °C (68 to 212 °F)	20 to 80 °C (68 to 176 °F)	0 to 150 °C (32 to 302 °F)	0 to 120 °C (32 to 248 °F)
	0 to 10 %	20 to 100 °C (68 to 212 °F)	20 to 80 °C (68 to 176 °F)	0 to 150 °C (32 to 302 °F)	0 to 120 °C (32 to 248 °F)

Index

A

Accessories	33
Air set	20
Ambient temperature	36
Approvals	18
Marine	19
Assembly	24

C

Cable extension	30
Calibration solutions	35
Cell constant	35
Certificates	18
Check	
Connection	30
Installation	24
Chemical resistance	41
Cleaning agent	31
Conductivity response time	36
Connection	
Check	30
Ensuring the degree of protection	30
Connection conditions	25

D

Declaration of Conformity	2, 18
Degree of protection	36
Ensuring	30
Designated use	9
Direct connection to transmitter	29
Disposal	33

E

Electrical connection	24
Environment	36
EU Declaration of Conformity	2
Ex approvals	18

F

Flange	21
------------------	----

H

Hazardous areas	10
---------------------------	----

I

Incoming acceptance	14
-------------------------------	----

Input	35
Installation	19
Installation conditions	19
Installation factor	19
Installation position	19
Interpreting the order code	17

L

Linearity	36
---------------------	----

M

Maintenance	31
Manufacturer's address	17
Marine	19
Materials	39
Maximum measured error	36
Measured variables	35
Measuring frequency	35
Measuring ranges	35
Mechanical construction	39

N

Nameplate	17
---------------------	----

O

Operational safety	10
------------------------------	----

P

Performance characteristics	36
Post-installation check	24
Pressure/temperature ratings	38
Process	37
Process connections	40
Process pressure	37
Process temperature	37
Product identification	14, 17
Product page	17
Product safety	10

R

Repair	32
Repeatability	36
Requirements for personnel	9
Return	33

S

Safety

Electrical equipment in hazardous areas . 10

Safety instructions 9

Scope of delivery 17

Sensor

Connecting 29

Connection in hazardous area 25

Mounting 21

State-of-the-art technology 10

Storage temperature 36

Symbols 7

T

Technical data 35

Environment 36

Mechanical construction 39

Performance characteristics 36

Process 37

Temperature measurement 35

Temperature response time 36

Temperature/pressure ratings 38

Type code 14

U

Use 9

W

Warnings 7

Weight 39

Wiring 29

Workplace safety 9



71464663

www.addresses.endress.com
