

GPR-x500 Oxygen Analyzers

User Manual PST-UM-3004-EN-03



Issue No.	Description	Date	Author Initials
01	Original document issued	01/2016	PP
02		02/2020	
03	* Re-brand template * Hazardous area information * New firmware information	02/2024	IM



GPR-x500 Oxygen Analyzers

For contact information, visit
ProcessSensing.com

Analytical Industries Inc (Aii) is part of the Process Sensing Technologies Group (PST). This document is the property of Process Sensing Technologies and may not be copied or otherwise reproduced, communicated to third parties, nor stored in any Data Processing System without the express written authorization of Process Sensing Technologies.

©2024 Process Sensing Technologies

Before using your GPR-x500

Safety information

Please read this manual, ensuring that you fully understand the content before attempting to setup, maintain or use the GPR-x500. Important safety information is highlighted throughout this document as follows:



The electrical warning symbol indicates instructions that must be followed to avoid serious or fatal injury from hazardous voltages and electric shock.



The warning symbol indicates instructions that must be followed to avoid minor, serious or even fatal injury to personnel.



The **electrostatic discharge (ESD) warning** symbol indicates the user must take precautions and follow the necessary steps to avoid generating electrostatic discharge.



The **caution** symbol indicates instructions that must be followed to avoid damage to equipment (hardware and/or software) or the occurrence of a system failure.

NOTE: Highlights an essential operating procedure, condition, or statement.

Abbreviations

AC	Alternating Current
DC	Direct Current
°C	Degrees celcius
°F	Degrees fahrenheit
EC	Electrochemical
ELV	Extra Low Voltage
ESD	Electrostatic Discharge
FSD	Full-scale Deflection
g	Grams
GND	Ground
IS	Intrinsically Safe
kg	Kilograms
lb	Pounds
LD	Liquid Drain
LDL	Lower Detection Limit
LED	Light Emitting Diode
LPM	Liters Per Minute
mA	Milliampere
OEM	Original Equipment Manufacturer
oz	Ounces
PC	Personal Computer
PCB	Printed Circuit Board
PLC	Programmable Logic Controller
ppb	Parts Per Billion
ppm	Parts Per Million
SCFH	Standard Cubic Feet per Hour
SS	Stainless Steel

Contents

Before using your GPR-x500	iii
Safety information	iii
Abbreviations	iv
1 Introduction	1
1.1 Overview	1
1.2 Models	2
1.3 Applications	2
1.4 Sensors	2
1.4.1 GPR-12-333 Sensor	3
1.4.2 -LD suffix Sensor	3
1.4.3 GPR-12-333-H Sensor	3
1.4.4 XLT-12-333 Sensor	3
1.4.5 GPR-11-60 Sensor	3
1.4.6 XLT-11-24 Sensor	3
1.5 Further general considerations	4
1.5.1 Conditions of use in hazardous areas	4
1.6 Safety approvals and directives	5
2 Installation	6
2.1 Unpack your analyzer	7
2.2 Analyzer features	8
2.3 Mount your analyzer	8
3 Connection	10
3.1 Connect your power supply	10
3.2 Hazardous area connections	11
4 Sensor installation	12
4.1 GPR-1500	12
4.2 GPR-2500	13
5 Before connecting gas	15
5.1 Necessary considerations before gas connection	15
5.2 Connect your gas	16
5.3 Calibration gases	16
5.4 Sample gas requirements	17
5.4.1 Inlet pressure	17
5.4.2 Outlet pressure	17
5.5 Prepare your zero/span gas	17
6 Operation	19
6.1 User interface	19
6.2 Initial start-up and self-test	20
6.3 Menus	21
6.3.1 Main Menu and interface keys	21
6.3.2 Range selection	22

6.3.3 Analyzer calibration 23

6.3.4 System 27

6.3.5 Info 29

7 Maintenance 30

7.1 Sensor replacement 30

7.2 Routine cleaning 30

7.3 Routine inspection of sensor housing 31

7.4 Troubleshooting 31

8 Warranty information 34

8.1 Coverage 34

8.2 Limitations 34

8.3 Exclusions 34

8.4 Service 35

9 Appendices 36

Appendix A - Technical Specifications 36

Appendix B - Hazardous Area Certification 37

Appendix C - Safety Data Sheet 38

Appendix D - Controlled Drawings 46

Appendix E - Mounting Information 47

Appendix F - Menu Displays 48

Appendix G - Spare Parts 49

Appendix H - Rating Plate 50

Appendix I - Quality, Recycling, and Warranty Information 51

1 Introduction

This user manual is applicable to the GPR-1500 and GPR-2500 oxygen analyzers.

! These products are for indoor and outdoor use. If they are used in a manner not specified by the manufacturer, the protection provided by this equipment may be impaired.

This document contains the following information for your analyzer:

- Installation
- Connection
- Operation
- Maintenance and troubleshooting.

To ensure that the latest manual is being used please visit the PST website www.processsensing.com.

Access the latest datasheets, user manuals, certificates and more at the product page **Downloads** tab.



GPR-1500



GPR-2500

1.1 Overview

GPR oxygen analyzers are reliable, compact, robust, and designed to perform verification measurements in a variety of industrial oxygen applications.

Features of GPR-1500 and GPR-2500 analyzers include:

- Simple, intuitive HMI
- Sensors available for measurement in CO₂ or H₂ gases
- User-selectable or automatic adjusted measurement ranges
- Gas temperature compensation
- Loop-powered configurations
- Range of sampling options available for different applications

1.2 Models

The GPR range of oxygen analyzers covered in this manual are detailed as follows:

- GPR-1500 - ppm oxygen online analyzer
- GPR-2500 - % oxygen online analyzer

These are loop-powered and certified for hazardous area installation.

1.3 Applications

- Monitoring inertization and blanketing gases for the storage or transport of hydrocarbons
- Monitoring natural gas quality
- Monitoring oxygen in pharmaceutical reactors and centrifuges.

1.4 Sensors

Our maintenance-free electrochemical sensors are galvanic cells capable of superior performance, accuracy and stability; designed to be unaffected by the presence of background gases. As a consumptive sensor type, it is disposable and requires only periodic calibrations.

Operational life is typically up to 18 months however, replacement frequency is dependent on the individual application.

If contaminants are present in the sample gas, the sensor can be affected, and the validity of the measurement impacted. Please ensure that the sensor is protected, and any contamination is prevented from reaching the analyzer's pipework and the sensor.

Consult the PST-Aii sales team about our cost-effective standard sample conditioning systems.

Table 1: Available sensor types:

Analyzer model	GPR-1500	GPR-2500	GPR-1500	GPR-2500
Model number	GPR-12-333 / GPR-12-333-LD / GPR-12-333-H	GPR-11-60 / GPR- 11-60-LD	XLT-12-333 / XLT- 12-333-LD	XLT-11-24 / XLT- 11-24-LD
Recommended O ₂ Measurement Range	0...1000 ppm _V	0...25 %	0...1000 ppm _V	0...25 %
Minimum Range	0...10 ppm _V	0...1 %	0...10 ppm _V	0...1 %
Sensitivity	0.01 ppm _V	0.005 %	0.01 ppm _V	0.005 %

For full sensor technical specifications, please refer to "Appendix A - Technical Specifications" on page 36.

1.4.1 GPR-12-333 Sensor

Our standard ppm sensor can be used to measure oxygen in a wide variety of gases.

Specific sensor selection should be given when the background gases are helium (He), hydrogen (H₂) or > 0.5 % carbon dioxide (CO₂).

1.4.2 -LD suffix Sensor

This is the standard sensor for use with sample gas containing occasional liquid. The LD sensor is in a screw-in housing and has a 4-pin molex process connection. The sensor itself is the same as standard.

1.4.3 GPR-12-333-H Sensor

In applications with a background gas of helium or hydrogen, we recommend using the -H sensor.

This sensor has the same construction as the standard sensor but a different electrolyte formula enables a quick measurement response with He and H₂ background gases.

1.4.4 XLT-12-333 Sensor

For measurement applications with ppm levels of oxygen in a background gas containing more than 0.5 % CO₂, the specially designed XLT sensor should be selected.

With most standard electrochemical sensors, an alkaline electrolyte is used; this is neutralized over time when exposed to acidic gases, such as CO₂. To combat this, Aii has developed the XLT sensor with a special electrolyte formula, which maintains functionality in temperatures as low as -10 °C.

1.4.5 GPR-11-60 Sensor

Our standard % sensor can be used to measure oxygen in a wide variety of gases.

1.4.6 XLT-11-24 Sensor

For measurement applications with % levels of oxygen in a background gas containing more than 0.5 % CO₂, the specially designed XLT sensor should be selected.

NOTE: Calibration is required each time your sensor is replaced. Ideally, your sensor should be replaced before reaching the end of its operational life.

1.5 Further general considerations

When your GPR-x500 analyzer is used with or in other equipment please consider the following:

- The analyzer should not be submerged in any liquid. Care should be taken to ensure liquids are not spilled and objects do not fall into the unit.
- Avoid force when using connectors, switches and knobs. Before moving your analyzer, be sure to disconnect the wiring/power cord and any cables connected to the output terminals.
- Ensure the sensor selected and supplied is suitable for the gas composition to which it will be presented; if in doubt, review the application and consult the PST-Aii Factory before initiating the installation.
- The products covered should be evaluated to the environmental conditions as defined by the standard up to 2000m altitude and within the temperature range applicable to your sensor; refer to "Appendix A - Technical Specifications" for details.
- The current rating and size of the power supply cable should be appropriate to the equipment.
- The products covered by this manual should be installed using the manufacturer's instructions.
- Only the sensor provided by the manufacturer is to be used with the analyzer.

NOTE: In natural gas applications such as extraction and transmission, a low voltage current is applied to the pipeline itself to inhibit corrosion of the pipeline. As a result, electronic devices connected to the pipeline can be affected unless they are adequately grounded.

1.5.1 Conditions of use in hazardous areas

NOTE: Always ensure the power is switched off prior to accessing the Ex enclosure for any purpose other than normal operation, or prior to disconnecting any cables.

Refer to "Appendix B - Hazardous Area Certification" on page 37 for certification details.

i) All versions of the enclosure are manufactured in aluminum. In rare cases, ignition sources due to impact and friction sparks could occur. This shall be considered during installation, particularly if the equipment is installed in a Zone 0 location.

ii) The online gas analyzers has non-metallic parts incorporated in the enclosure of this equipment which may generate an ignition-capable level of electrostatic charge, under certain extreme circumstances. Therefore, the equipment shall not be installed in a location where the external conditions are conducive to the build-up of electrostatic charge on such surfaces. This is particularly important if the equipment is installed in a Zone 0 location. In addition, the equipment shall only be cleaned with a damp cloth.

iii) The online gas analyzer is not capable of withstanding the 500 V insulation test required by Clause 6.3.12 of IEC 60079-11. This shall be taken into account when installing the equipment.

iv) When connected using a conduit system, the explosion-proof enclosures type Adalet type XIHLX require conduit seals.

v) When connected with cable glands, the glands shall be a suitably Listed Explosion-proof type, suitable for the applicable Class and Division or Class and Zone, Gas Group, T-Class and ambient

temperature. It shall only employ sealing around individual cores. Additional thread adapters shall not be used.

1.6 Safety approvals and directives



The CE marking indicates GPR-x500 oxygen analyzer conformity to European health, safety, safety and environmental protection directives.



The Ex marking indicates GPR-x500 oxygen analyzer conformity to European Union directive 2014/34/EU (ATEX) and UK Statutory Instrument 2016 No. 1107 (as amended) (UKEX). It complies with Intrinsically Safe (I.S) standards for equipment category 2 when used following the instructions for safe use in this user manual. This makes it normally suitable for use in Zones 1 or 2 hazardous areas.



This UKCA marking demonstrates GPR-x500 oxygen analyzer complies with UK designated standards in electric and electronic engineering and measuring technology.



The MET marking certifies GPR-x500 oxygen analyzer is compliant in North America and Canada, with the electrical and hazardous location safety directive.

NOTE: The GPR-x500 range of analyzers are not tri-rated. These analyzers are built to comply with ATEX / IECEx / UKEX or cMETus. The hazardous area compliance rating is shown on the rating plate on the analyzer. Please ensure your analyzer is compliant with site or location requirements. This manual details installation, operation and support for all GPR-x500 analyzers for all certifications.

2 Installation

NOTE: Installation, operation and maintenance of this equipment should be carried out only by appropriately trained and suitably qualified technicians in accordance with the instructions in this user manual, and any applicable standards/certificates associated with the country, industry and application.



Failure to correctly adhere to these instructions may result in serious or even fatal injury. In this regard, the manufacturer will not be held liable.

NOTE: The operator may only perform modifications and repairs to the equipment or system with approval from the manufacturer.



Do not operate damaged equipment. If faults cannot be rectified, the equipment must be taken out of service and secured against unintentional commissioning.

Before using your GPR-x500, ensure that its specifications are suitable for the process in which it will be installed.

2.1 Unpack your analyzer

If sold separately (not part of a sampling system), the GPR-x500 will be supplied in a custom box which should be retained for future use (such as a service return).

Your GPR-x500 analyzer pack is comprised of the following equipment (pack contents may vary depending on your specification):


1. GPR-x500 analyzer
2. Sensor (in double-foil pack)
3. Remote barrier (supplied with hazardous area models)
4. PST-Aii Factory calibration certificate
5. Quick Start Guides (ref: PST-QSG-3205, span calibration, PST-QSG-3206, air calibration)
6. User Manual, this document (ref: PST-UM-3004) on a USB stick.



Figure 1. Contents of GPR-x500 pack

2.2 Analyzer features

The GPR-x500 analyzer consists of two interconnected enclosures enclosures (without the optional sample conditioning system and panel) and measures 8.4" (L) x 4.4" (W) x 10" (H).

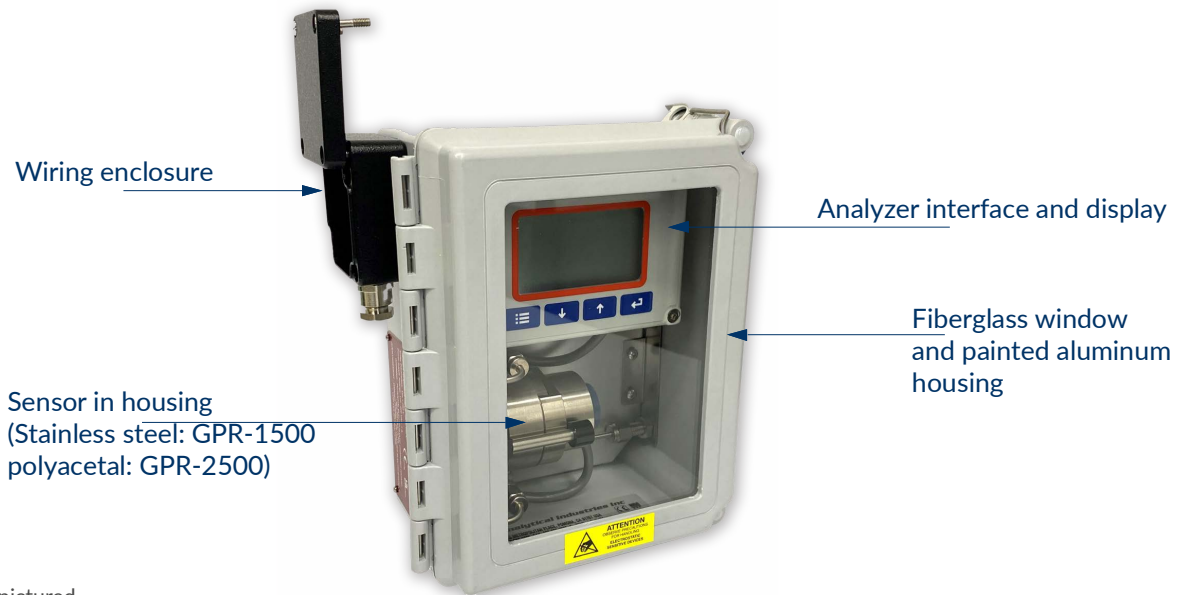

GPR-1500 pictured

Figure 2. The GPR-x500 oxygen analyzer set-up

2.3 Mount your analyzer

The analyzer is approved for indoor as well as outdoor use. However, avoid mounting in an area where direct sun might heat up the analyzer beyond the recommended operating temperature range. If possible, install a small hood over the analyzer for rain water drain and to prevent over-heating of analyzer.

- Find the appropriate location to install the analyzer.
- Ensure that the mounting and operation is only in the upright vertical orientation.
- To facilitate convenient servicing the interior of the transmitters, secure the back plate to a vertical surface approximately 1.5 m (5 ft) from the floor or a level accessible to service personnel. This requires the user to supply four (4) additional proper sized screws and anchors.

NOTE: For installations where temperature can be expected to fall below -18 °C (0 °F) please consult PST-Aii Sales to discuss heated enclosure options.

This GPR-x500 configuration is designed to be mounted directly to any flat vertical surface, wall or bulkhead plate. Please see "Appendix E - Mounting Information" on page 47.

The analyzer's design provides immunity from RFI/EMI by maintaining good conductive contact between the two halves of the enclosures via a conductive gasket (the smaller enclosure containing signal processing electronics).

The surfaces contacting the conductive gasket are unpainted. Do not paint these areas. Painting will negate the RFI/EMI protection.



Do not remove or discard the gaskets from either the Ex enclosure or the fiberglass enclosure. Failure to reinstall either of the gaskets will void the NEMA 4, UL Type 3R rating and the immunity to RFI/EMI.

For mounting requirements and information, please refer to "Appendix E - Mounting Information" on page 47.

3 Connection

Supply power to the analyzer only as rated by the specification or markings on the analyzer enclosure. The wiring that connects the analyzer to the power source should be installed in accordance with recognized electrical standards.

Ensure that the analyzer case is properly grounded and meets the requirements for area classification where the analyzer is installed. Never use force when removing wiring from a terminal connection.

3.1 Connect your power supply

This configuration is **loop-powered**; it requires a 18...24 V DC power supply on a 4...20 mA loop.

Incoming power is connected via a 3-way terminal block.

 Do not supply voltage more than specified in this manual and noted near the power input terminal of the analyzer.

 Do not apply line-power to the GPR-1500 or the GPR-2500. If line-power is applied to a loop-powered analyzer, it will result in damage to the main PCB.

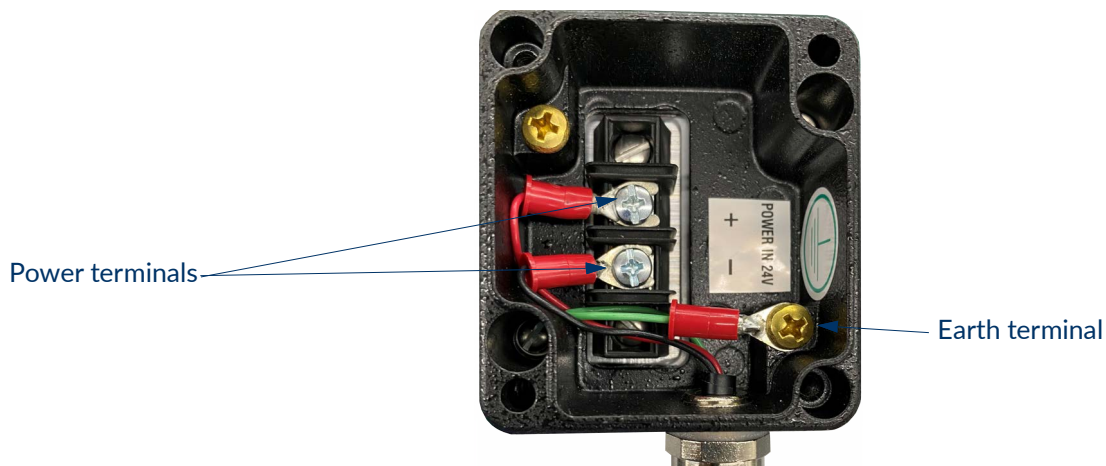


Figure 3. Wiring and connections

The maximum power consumption for GPR-x500 analyzers is 1.8 W.

3.2 Hazardous area connections

For installation in a hazardous area:

- Entity parameters for all connection facilities are as follows:
 - o **Ui = 28 V DC, li = 93 mA**
- All cables must be shielded to ground at customer side.
- Use a certified cable gland or stopper box.
- The power cable to the Ex enclosure must be supplied through a conduit approved for use in hazardous areas.
- Secure the wires to the power input terminal block by using the integral screws of the terminal block. Do not substitute terminal screws.

4 Sensor installation

NOTE: Please read through this procedure and "5 Before connecting gas" on page 15 before attempting to install your sensor.

4.1 GPR-1500

The GPR-1500 oxygen analyzer is equipped with stainless steel sensor housing. This housing offers ease of replacement of sensor whilst preventing any leakage into the system. The two sections of the sensor are held together by a metal clamp secured in place by an easily accessed bolt.

The integrity of the sensor housing has been tested at the PST-Aii Factory prior to shipment.

The analyzer must be calibrated once the installation has been completed and periodically thereafter.

To install or replace an oxygen sensor:

1. Apply power to your analyzer (refer to Figure 3 on page 10 for guidance).
2. Using the two latches, open the front window of the enclosure.
3. Open the sensor housing (refer to [Figure 4](#) below for guidance).

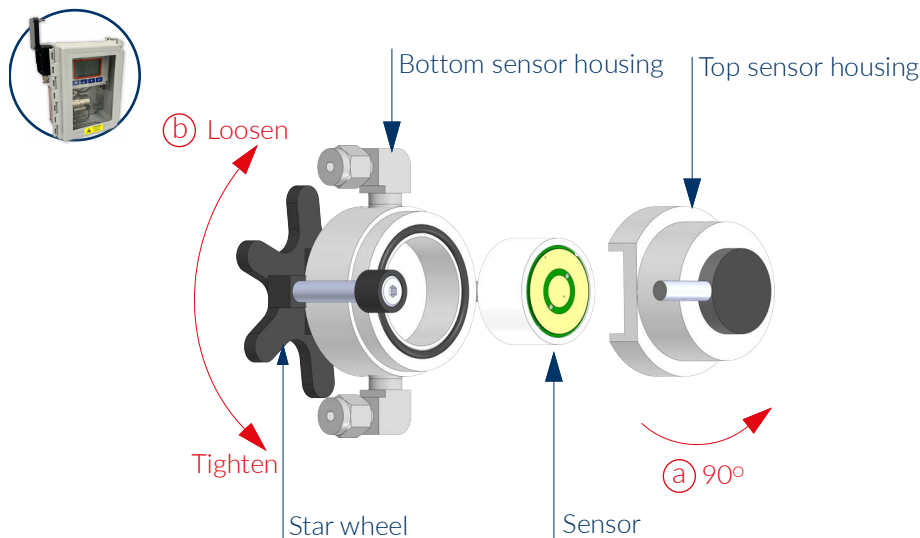


Figure 4. Installing and uninstalling your sensor (GPR-1500)

4. Loosen the star wheel then disengage the top sensor housing by turning it 90° counter-clockwise.
5. If replacing your sensor, remove the old sensor from the sensor housing, otherwise continue to the next step.

6. Remove the sensor from its packaging, remove the shorting flags and immediately place in the top sensor housing with the gold contact plate facing towards two gold contact pins in the top sensor housing as shown in [Figure 5](#).



Figure 5. Aligning your sensor

7. You may perform a zero and span calibration or an air calibration to confirm that the sensor output is within the recommended limits. See "Zero and span vs span calibration" on page 24 and for guidance.
8. Secure it with the star wheel at the bottom of the housing assembly (refer to 'b' in Figure 4 on page 12).
9. Quickly close your analyzer and connect your process sample gas or zero oxygen gas immediately.




Always minimize the time that the sensor is exposed to ambient air.

4.2 GPR-2500

The GPR-2500 analyzer is delivered with the sensor installed. If you need to replace your sensor, follow the procedure below.

1. Apply power to your analyzer
2. Using the two latches, open the front window of the enclosure.
3. Open the sensor housing (refer to [Figure 6](#) below for guidance).

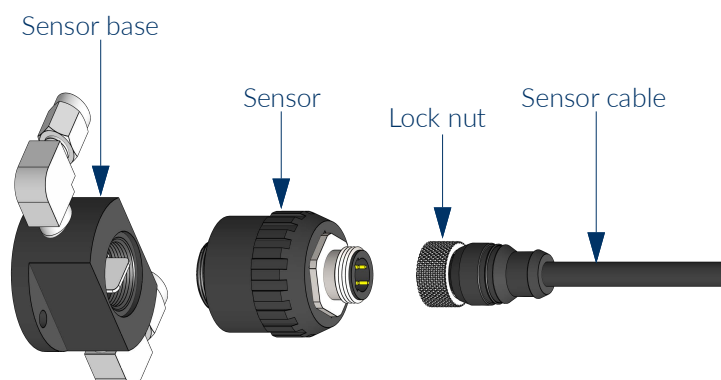

Sensor appearance may vary depending on your configuration

Figure 6. Installing and uninstalling your sensor (GPR-2500)

4. Disconnect the sensor cable by turning the lock nut counter-clockwise and unscrewing the old sensor from the sensor base.
5. Remove the new sensor from its packaging, remove the shorting flags and immediately screw it into the sensor base.
6. Secure the sensor cable by turning the lock nut clockwise.
7. Quickly close your analyzer and connect your process sample gas or zero oxygen gas immediately, following the procedure in "5.2 Connect your gas" on page 16.

5 Before connecting gas

5.1 Necessary considerations before gas connection

With standard flow-through configuration, the GPR-x500 analyzers are designed for positive pressure samples and require connections for incoming sample and outgoing vent lines.

Your analyzer is equipped with two gas ports as shown in [Figure 7](#).

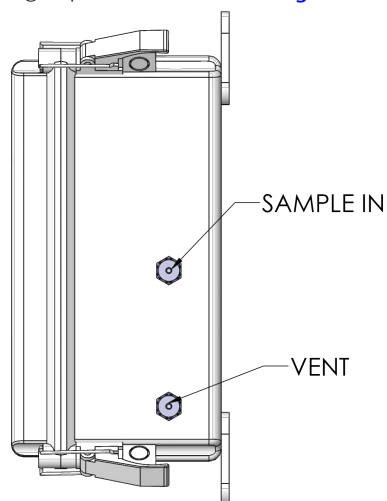


Figure 7. Gas ports (right elevation)

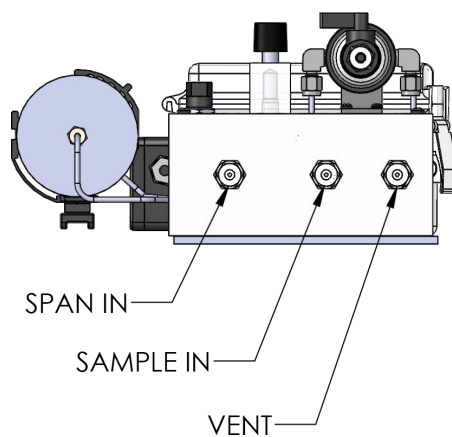


Figure 8. Gas ports: sample system (bottom elevation)

The inlet and outlet vent gas lines require 1/4" stainless steel compression type tube fittings.

The sample inlet tubing must be metallic, preferably stainless steel (SS). The sample vent line may be of SS or hard plastic tubing with low gas permeability.

To ensure the best possible operation, a review of the installation is recommended:

- a. Sample gas quality
 - Is the sensor suitable for gas?
 - Is a gas scrubber required?
 - Is the sample gas clean and liquid free?
- b. Stainless steel tubing (essential for maintaining the integrity of the gas stream for very low ppm or % level analysis).

NOTE: If operated in potentially contaminated gases, which can interfere with measurement and reduce the sensor's life expectancy. Consult PST-Aii for recommendations concerning the proper selection and installation of components.

5.2 Connect your gas

To connect your gas:

1. See [Figure 7 on page 15](#) for port designation and connect your **Sample** and **Vent** lines accordingly.
2. Regulate the sample pressure as described in below in "5.3 Calibration gases".
3. Connect a 1/8" or 1/4" vent line to the compression fitting to be used for venting the sample.
4. Connect a 1/8" or 1/4" sample line to the compression fitting to be used to bring sample gas to the analyzer.
5. Set the **Sample** gas pressure between 5...30 psi (0.4...2.1 bar).
6. Select sample gas and allow it to flow through the analyzers and set the flow rate to 1...2 SCFH (0.5...1 LPM).

Zero and span calibration gas ports are offered as part of the optional sample systems.

NOTE: If the analyzer is equipped with an optional H₂S scrubber, sample inlet pressure must not exceed 30 psi (2.1 bar).



Do not place your finger over the vent (it pressurizes the sensor) to test the flow indicator when gas is flowing to the sensor. Removing your finger (the restriction) generates a vacuum on the sensor and may damage the sensor, voiding the sensor warranty.

5.3 Calibration gases

NOTE: It is recommended that you use a certified zero and span gases for calibration to ensure the best measurement readings.

Cylinders of the appropriate certified zero and span gases should be made available for installation and commissioning. Calibration gases will need to be set to the same input pressure and flow rate as the sample gas to ensure calibration integrity.

5.4 Sample gas requirements

All gas analyzers utilizing electrochemical oxygen sensors respond to partial pressure changes in oxygen. To ensure accurate measurement of the oxygen sample, gas must be presented to the analyzer at a stable pressure and flow rate.

5.4.1 Inlet pressure

For the analyzers designed to measure oxygen in a flowing gas stream, the inlet sample pressure must be regulated in the range 5...30 psi (0.4...2.1 bar).

5.4.2 Outlet pressure

The sample must be vented at a pressure less than the inlet pressure so that the sample gas can flow through the sensor housing. Ideally, the sample should be vented to the atmosphere or into a flare at atmospheric pressure.

NOTE: The sensor may be used at a slightly positive pressure (e.g., when sample is vented to a common exhaust where the pressure might be higher than 1 atmosphere). However, the pressure at the sensor must remain constant at all times including during the span calibration. This may be accomplished by using a back-pressure regulator on the vent line of the analyzer.

If assistance is required to configure a measurement at a positive pressure, please contact PST-Aii with full application details for a review.



A sudden change in pressure at the sensor may result in the sensor electrolyte leakage.

5.5 Prepare your zero/span gas

Avoid contamination of the zero/span gas cylinder when connecting the pressure regulator. Bleed the air-filled regulator for a couple of minutes before closing the vent valve of the pressure regulator (faster and more reliable method of purging the regulator than simply allowing the zero/span gas to flow through the regulator and the span gas line).

The following components/tools are required to set up a zero/span gas cylinder:

- Certified zero/span gas cylinder with an oxygen concentration, balance nitrogen, of approximately 80 % of the full scale range above the intended measuring range.
- A pressure regulator to enable reduction of gas pressure to between 5 and 30 psi (0.4...2.1 bar).
- A flow meter (for use only if the analyzer is not equipped with one) to set the flow rate between 1 and 2 SCFH (0.5...1 LPM).
- Suitable fittings and 1/8" diameter metal tubing to connect the regulator to the inlet of the analyzer.

Ensure your zero/span gas cylinder valve is closed, then:

- Install the regulator on the cylinder using good practice.
- Open the regulator's exit valve and partially open the pressure regulator's control knob.

3. Slightly open the cylinder valve.
4. Loosen the nut connecting the regulator to the cylinder and bleed the pressure regulator.
5. Re-tighten the nut connecting the regulator to the cylinder.
6. Adjust the regulator exit valve and slowly bleed the pressure regulator.
7. Open the cylinder valve completely.
8. Set the output pressure between 5 and 30 psi using the pressure regulator's control knob.



Do not exceed the recommended pressure. Excessive pressure will make flow adjustment more difficult.

6 **Operation**

This section details the best practice operation for a correctly installed analyzer. Please refer to "2 Installation" on page 6 for analyzer installation guidance and gas connection.

6.1 **User interface**

The GPR-x500 has a 1-inch LCD display and a four-key keypad interface.

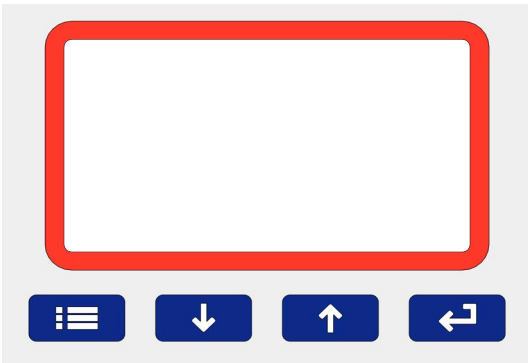


Figure 9. GPR-x500 user interface

The interface keys can be used as identified in the table below:

Table 2: Interface key functions

Key	Function
	Menu open/close
	Enter
	Next (increment)
	Previous (decrement)

6.2 Initial start-up and self-test

Once the analyzer is correctly installed and power applied the analyzer will immediately start up. The digital display responds instantaneously and will display an initial start-up screen:



Figure 10. GPR-series analyzer start-up screen

After self-diagnostic tests, the analyzer switches to sampling mode and displays the oxygen reading from the sensor (larger size numeric value) and the measurement range (small size font with units).

Auto indicates that the analyzer is in AUTO mode. In this mode, the measured value affects the range, which will automatically adjust to the next higher level. See **Range** (page 22) in the **Main Menu** to select.

If the **Auto** is not selected, the range display will not show **Auto**. An example of a sampling mode screen is shown below in [Figure 11](#).

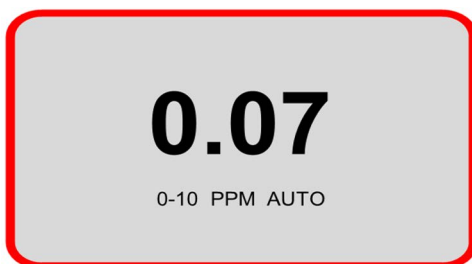


Figure 11. Measurement mode display

6.3 Menus

NOTE: Available menu options and sequences will vary between analyzer model and sensor type.

6.3.1 Main Menu and interface keys

To access the Main Menu, press the **Menu** key and the following Main Menu display will appear:

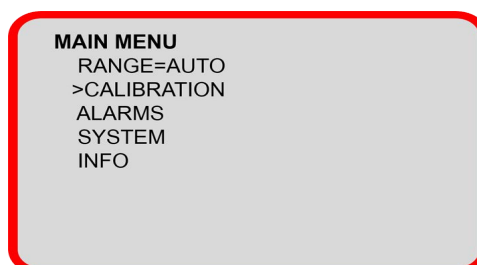


Figure 12. Main menu display

This screen shows the menu options available.

- Use the  and  keys to move the cursor to the desired menu
- Press  to access the sub menu
- Use the  key to return to the previous screen.

Range

Configure analyzer measurement range (see "6.3.2 Range selection").

Calibration

Perform zero, span or analog calibration functions (see "Zero and span vs span calibration" on page 24).

System

Configure system-level settings (see "6.3.4 System" on page 27).

Info

View analyzer information (see "6.3.5 Info" on page 29).

6.3.2 Range selection

Within the Range menu, you can select 6 options. The range is linked to the display and the 4...20 mA analog output of the analyzer.

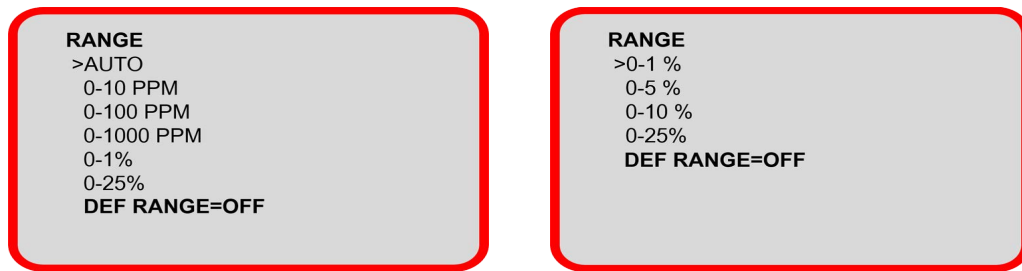


Figure 13. GPR-x500 Range displays

NOTE: For trace oxygen analyzers, the range 0...25 % is for calibration purposes only. It is not a measurement range of the analyzer (see " Zero and span vs span calibration" on page 24 for calibration). Using this range extensively can significantly shorten the sensor life.

Range menu options

In the Range menu:

1. Use  and  to move the cursor to the desired range option.
2. Once the cursor is pointing to your chosen range, press  to select the range.

Selecting a range will cause the **Auto** option to change to **Fixed**. To select Auto, use  to move the cursor to **Fixed**, then press  to toggle between **Auto** and **Fixed**.

Auto

Selecting **Auto** will enable automatic adjustment of your measurement range depending on the oxygen levels detected by your oxygen sensor. For example, a 0...10 ppm range will change to 0...100 ppm if the measured oxygen value is higher than 10 ppm.

Default Range

This option will prevent incorrect range-setting if multiple users have access to the analyzer.

If the analyzer range has been changed, for instance for the purpose of checks or maintenance, and a default range has been pre-set, the analyzer will automatically return to the default range after 30 minutes of inactivity.

Def Range allows you to set the default range for the analyzer. Within this sub-menu, all standard ranges or **Auto** mode can be selected.

It is recommended that you set your preferred default range for the analyzer.

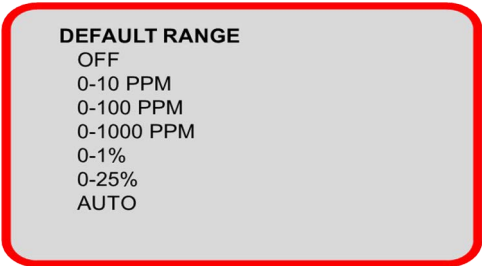


Figure 14. Default Range display

Measurements outside manual range

If the oxygen reading goes above the manual or auto range maximum value, the values will be displayed up to 10% above the maximum range. Beyond this, an OVER RANGE warning will be displayed.

6.3.3 Analyzer calibration

All electrochemical sensor-based analyzers require periodic calibration. The electrochemical sensor signal will remain relatively constant throughout its useful life, however, some components in a gas stream, e.g. sulfides, can adversely affect the sensor causing changes in sensitivity with time. As such, regular calibration is recommended to ensure accuracy and ascertain the integrity of the sensor (e.g. weekly intervals to a 3-month maximum).

Always use good calibration practices.

- Calibrate the analyzer at or close to the temperature and pressure of the sample gas.
- Use known reference gases or fresh air.
- Allow suitable stability time especially when making significant changes in measurement value (e.g. 20.9 % to 0.0 %). Use the table below for guidance.

Table 3: Example stability times

Condition example	Typical stability time
<1 % to air (20.9 %)	<3 minutes
Air (20.9 %) to 0.1%	<30 seconds
Air (20.9 %) to 0.01%	<2 minutes
2 minute air exposure to 10 ppm	60 minutes

Set sensor serial

Updating the sensor serial number is critical for the calibration process.

When replacing O₂ sensors it is important to update the sensor serial number. To view the current 9-digit sensor serial number, enter the **Calibration** menu.

The sensor serial number can be seen in the menu as shown below:



Figure 15. Calibration display

NOTE: Changing the sensor serial number will reset span and zero calibrations to Factory defaults and clear the calibration log. It should only be changed when a new sensor is installed.

To change the sensor serial number:

1. Use  to select **Sensor SN=00000000**.
The display will change as shown below in [Figure 16](#).

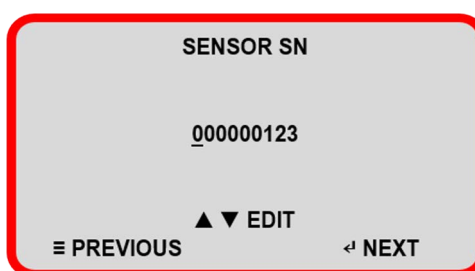


Figure 16. Sensor serial number display

2. Enter your sensor serial number by using  or  to edit the value.
3. Press  to progress to the next digit or  to move to the previous digit.
4. When you have entered your sensor serial number's last digit, press  to **Accept** the new serial number.

Zero and span vs span calibration

Electrochemical oxygen sensors generate an electrical current that is linear or proportional to the oxygen concentration in a sample gas. In the absence of oxygen the sensor exhibits an absolute zero, i.e. the sensor does not generate a current output in the absence of oxygen. Given the properties of linearity and an absolute zero, a single point calibration is possible.

Zero calibration is recommended only when the application demands optimum accuracy of better than 5 % of the lowest range of the analyzer (e.g. for an analyzer configured for 0...25 % range, we would recommend a zero calibration if measurements below 1.0 % O₂ were required).

Span calibration is required routinely for accurate measurements of oxygen.

NOTE: Zero calibration should always be carried out before a span calibration.

Zero calibration

The zero calibration adjustments are limited to 30 % of the most sensitive range. All analyzers are QC-tested to confirm the zero calibration. Should you observe a zero calibration error more than 30 % of the lowest range, we recommend first:

- Check the sample system for any possible leaks
- Confirm the integrity of the zero gas
- Ensure the analyzer has been given enough time to stabilize on the zero gas
- Ensure CLIP = OFF, refer to "Clipping" on page 28 for information.

If adequate time is not allowed for the analyzer to establish the true baseline and a ZERO calibration is performed, the analyzer will likely display a negative reading in the sample mode when exposed to zero gas. If a negative reading is observed, we recommend repeating the ZERO calibration.

To perform a zero calibration:

1. Enter the **Calibration** menu and select **Zero Calibrate**.
The analyzer will switch to **Zero Cal** mode and display the live readings.

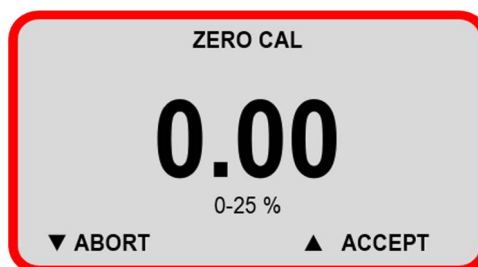


Figure 17. Zero calibration display

2. Once gas readings are stable you can **Accept** or **Abort** the calibration.
The calibration will **Pass** or **Fail** and the analyzer will return to normal operation at the configured range.

During calibration ensure stability of readings, secure gas connections and supply of suitable reference gas.

Span calibration

To perform a Span Calibration, enter the **Calibration** menu and select **Span Calibration**.

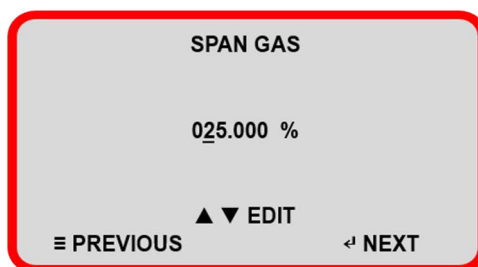


Figure 18. Span gas display

In the sub-menu, set the Span Gas value. If using certified cylinder gas, this can be found on the certificate that was supplied with the cylinder:

1. Use  to progress to the next digit or  to move to the previous digit; use  and  to edit the values.

NOTE: When a Span or Zero Cal starts, only "Abort" with  is shown until the reading is stable, then "Accept" with  appears.

2. Now select the unit in use (% or ppm).
3. When you press , the analyzer will switch to the appropriate range and display the live readings.

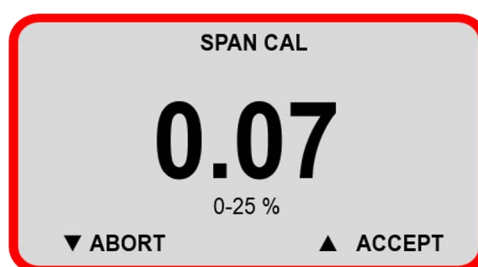


Figure 19. Span calibration display

Once gas readings are stable you can **Accept** or **Abort** the calibration. The calibration will **Pass** or **Fail** and the analyzer will return to normal operation at the configured range.

During calibration ensure stability of readings, secure gas connections and supply of suitable reference gas.

NOTE: If using a ppm sensor we do not recommend exposure of the sensor to ambient air as it will significantly degrade the sensor life.

Calibration log

The Cal Log shows a summary of events on the analyzer. A total 256 records can be recorded.

Details included are shown below;

Date	Cal Type	Correction Value	Pass/Fail
01/01/23	RST		
01/01/23	SPN	-0.05	P
01/01/23	ZRO	-1.00	F

ZRO =	Zero calibration
SPN =	Span calibration
RST =	Reset calibration to factory calibration

NOTE: The correction value does not relate to actual readings it is a proportional value. This value can be used by the PST Factory for diagnostics.

6.3.4 System

Use the System menu to make the system adjustments shown in [Figure 20](#).

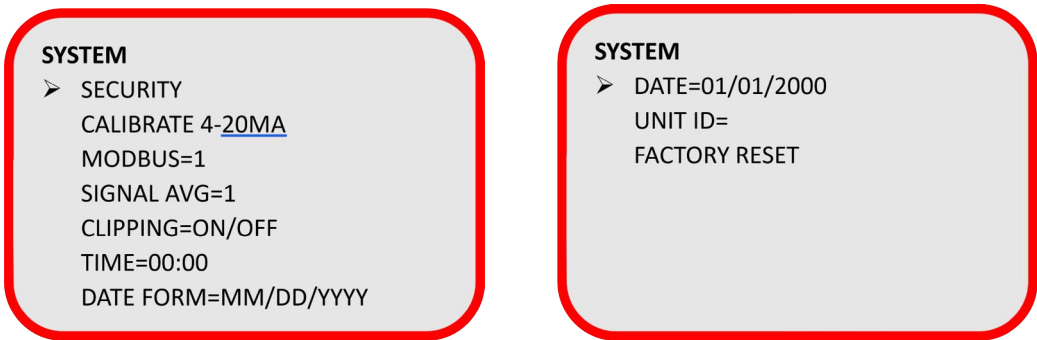


Figure 20. System display

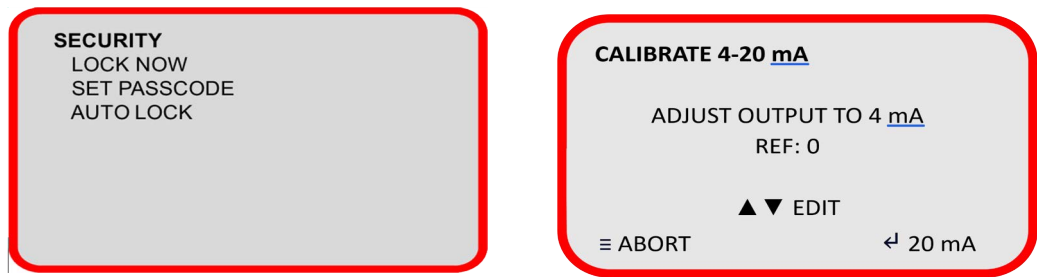


Figure 21. System sub-menu displays

Security

- Enable Screen Lock with a passcode (default code is 0000)
- Set Passcode > Set the 4-digit passcode
- Enable Auto Lock > Locks the screen after 30 minutes.

Calibrate 4...20 mA

This sub-menu allows a direct offset to be applied to the 4...20 mA analog output.

1. Use the keypad to adjust the reference corrections for both 4 and 20 mA outputs.
2. Select **Accept** to apply the adjustments or **Abort**.

Signal AV - signal average

This function enables the setup of a measurement rolling average. A value between 1...100 readings can be used in a simple average calculation for the display measurements. Measurements are made at 1 Hz so that a value of 60 will give a 1-minute rolling average.

Higher signal average will help remove measurement instability but will reduce measurement response.

Clipping

Enabling Clipping will stop the analyzer displaying below 0 ppm / 0 % readings.

Time

Sets the on board 24-hour clock for data logging.

Date form

This user-configurable functions enables you to set your date format preference to one of the following:

mm/dd/yy
dd/mm/yy
yy/mm/dd

Date

Set the on board device date (after a full power cycle the date time will be 00:00 1 Jan 2000).

Range scale

Adjusts the ppm range max value by a multiple (1-5).

For example setting Range Scale to 5 will give the following Range Options in the **Range** menu:

- 0-50 ppm
- 0-500 ppm
- 0-5000 ppm

Your analyzer is supplied with a Range scale of 1 as standard. This will generate ranges of:

- 0-10 ppm
- 0-100 ppm
- 0-1000

NOTE: Range scale only applies to the lowest three ranges of group 1 O₂ (10, 100, 1000 ppm O₂).

Unit ID

Allows an Alpha numeric ID to be given to the analyzer. This value will be stamped on log files and displayed on the INFO SCREEN.

Factory reset

Reverts all settings to Factory Configuration including security settings, sensor calibration and analog calibration.

6.3.5 Info

The **Info** menu displays the device information including:

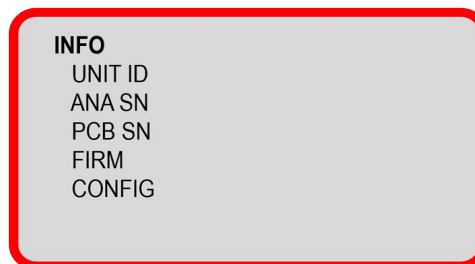


Figure 22. Info display

- **UNIT ID:** User defined (this is left blank for user, usually a location ID or asset number is entered here)
- **ANA SN:** Serial number of the analyzer (The 9-digit analyzer serial number is also displayed in log files)
- **PCB SN:** Serial number of the circuit board (a 9-digit number)
- **FIRM:** Firmware part number and revision
- **CONFIG:** This number refers to your analyzer's power, gas and Factory group number.

7 Maintenance

The GPR-x500 will provide reliable and fault-free service with regular maintenance and calibration.

During periods without use the sensor should be purged with nitrogen or argon gas to preserve the sensor life.



Do not attempt to make repairs to the analyzer. This will void the warranty and may result in electrical shock, injury, or damage. All servicing should be referred to qualified service personnel.

7.1 Sensor replacement

To maintain performance, the sensor in your GPR-x500 analyzer will require replacement. Sensor life is application dependent.

When your sensor reaches the end of its serviceable life, calibration can no longer be performed and the sensor must be replaced.

A regular program of calibration will mitigate against sudden sensor failure. It is advisable to establish a program of preventative maintenance to ensure process downtime is kept to a minimum or avoided.

The protective plugs on your sensor should only be removed when your GPR-x500 is installed and ready to begin gas measurement.

Refer to "5 Before connecting gas" on page 15 for the sensor installation procedure.

7.2 Routine cleaning

During sensor replacement, it is recommended that light cleaning of electrical contacts is carried out.



Never use chemical cleaning agents, solvents or high pressure water or steam to clean the equipment. Do not submerge in water.

To perform routine cleaning:

1. Use a clean cloth that is damp with water to wipe away dust and dirt from the outside of the unit.
2. Dry the analyzer with a clean, dry cloth.

7.3 Routine inspection of sensor housing

The maximum interval between routine inspections should be determined with consideration of the application and importance of the measurement.

The interval should be reassessed on a regular basis and can be extended and reduced as the process control requires.

This can be carried out during sensor replacement. To perform routine inspection:

1. Ensure the gas entry and vent ports on the sensor housing are not obstructed.
2. Inspect the sensor housing seal and replace it if damage is visible.

7.4 Troubleshooting

- Ensure the correct calibration gas is used when performing a validation or calibration of your analyzer. This will prevent unpredictable operation and incorrect readings.
- The calibration gas should be within range of your GPR-x500, typically 100 ppm for the 0...1 % range analyzer, and 20.9 % for the 0...25 %. See the PST Factory calibration certificate supplied with your module for specific calibration gas values.
- A faulty sensor or one that is incorrectly installed will display 'FLT' on your analyzer's display.
- Do not expose the sensor to moisture in an un-powered state. If this happens, allow the sensor to dry out, and if necessary, apply clean dry inert gas.

Table 4: Troubleshooting causes and recommendations

Symptoms	Possible cause	Recommended actions
Slow recovery.	At installation, defective sensor.	Replace sensor if recovery unacceptable or O ₂ reading fails to reach 10 % of lowest range.
	Air leak in sample system connection(s).	Leak test the entire sample system: Vary the flow rate, if the O ₂ reading changes inversely with the change in flow rate indicates an air leak - correct source of leak.
	Abnormality in zero gas.	Qualify with zero gas. Replace sensor.
	Damaged in service - prolonged exposure to air, electrolyte leak.	Replace sensor.
	Sensor nearing end of life.	Replace sensor.
High O ₂ reading after installing or replacing sensor.	Analyzer calibrated before sensor stabilized caused by:	
	Prolonged exposure to ambient air, worse if sensor was left in air un-shorted.	Allow O ₂ reading to stabilize before making any calibration adjustment, continue purge with zero gas.
	Air leak in sample system connection(s).	Leak test the entire sample system (above).
	Abnormality in zero gas.	Qualify with zero gas.
High O ₂ reading sampling.	Flow rate exceeds limits Pressurized sensor.	Correct pressure and flow rate. Remove restriction on vent line or open.
	Improper sensor selection.	SHUT OFF valve completely. Replace GPR/PSR sensor with XLT sensor when CO ₂ or acid gases are present. Replace GPR/PSR sensor with -H sensor when H ₂ or He gas is the background gas.
	Abnormality in sample gas measurement.	Validate with portable oxygen analyzer.
Response time slow.	Air leak, dead legs, longer distance of sample line, low flow rate, high volume of optional filters and scrubbers.	Leak test sample system bringing sample gas to analyzer, reduce dead volume and/or increase sample flow rate.
O ₂ reading doesn't agree with expected O ₂ values.	Pressure and temperature of the sample may be different than the span gas used for calibration Abnormality in the sample gas.	Calibrate the analyzer (calibrate close to the pressure and temperature of the sample gas).
		Qualify sample gas independently.

Symptoms	Possible cause	Recommended actions
Erratic O ₂ reading or No O ₂ reading.	Test sensor signal output independent from analyzer.	Remove sensor from housing. Using a volt-meter set to uA output, apply the (+) lead to the outer ring of the sensor PCB and the (-) lead to the center circle to obtain the sensor's output in air. If no current signal, replace sensor, otherwise contact the PST Factory.
	Abrupt changes in sample pressure.	Regulate sample gas pressure and flow.
	Dirty electrical contacts in upper section of sensor housing.	Replace sensor.
	Corroded solder joints on sensor PCB from corrosive sample or electrolyte leakage from sensor Corroded spring loaded contact in upper section of sensor housing from liquid in sample or electrolyte leakage from sensor.	Clean spring loaded contacts in upper section of sensor housing with a damp cloth or cotton swab, water or IPA can be used. If electrolyte leakage from sensor is evident, replace sensor.
	Liquid in sensor housing.	Wipe sensor and sensor housing with a damp cloth or cotton swab. Water or IPA can be used.
	Improper sensor selection.	Replace GPR/PSR series sensor with XLT sensor when CO ₂ or acid gases are present.
	Presence of other interference gases.	Consult PST Factory.
	Presence of sulfur gases.	Replace sensor and install H ₂ S scrubber.
	Unauthorized maintenance.	Replace sensor, obtain authorized service.
Erratic O ₂ reading or Negative O ₂ reading or No O ₂ reading possibly accompanied by electrolyte leakage.	Sensor nearing end of life.	Replace sensor.
	Pressurizing of the sensor by flowing gas to the sensor with the vent restricted	Zero the analyzer. If not successful replace the sensor.
	Pressurizing of the sensor by flowing gas to the sensor with SHUT OFF valve closed then suddenly removing the restriction to draw a vacuum on the sensor, or partially opening the valves upstream of the analyzer when using a pump downstream of the analyzer to draw sample from a process at atmospheric pressure or a slight vacuum.	Avoid drawing a vacuum on the sensor.
	A pressurized sensor may not leak but still can produce negative readings.	
	Placing a vacuum on the sensor in excess 40" of water column is strongly discouraged.	
	A premature ZERO OFFSET of analyzer.	From MAIN MENU select DEFAULT ZERO and perform a zero calibration.

8 Warranty information

The design and manufacture of Analytical Industries Inc. oxygen analyzers and oxygen sensors are performed under a certified Quality Assurance System that conforms to established standards and incorporates state of the art materials and components for superior performance and minimal cost of ownership.

Prior to shipment every analyzer is thoroughly tested by the manufacturer and documented in the form of a Quality Control Certification that is included in the Owner's Manual accompanying every analyzer.

When operated and maintained in accordance with the Owner's Manual, the units will provide many years of reliable service.

8.1 Coverage

Under normal operating conditions, the analyzers and sensors are warranted to be free of defects in materials and workmanship for the period specified in accordance with the most recent published specifications, said period begins with the date of shipment by the manufacturer.

The manufacturer information and serial number of this analyzer are located on the rear of the analyzer. Analytical Industries Inc. reserves the right in its sole discretion to invalidate this warranty if the serial number does not appear on the analyzer.

If your Analytical Industries Inc. monitor, analyzer and/or oxygen sensor is determined to be defective with respect to material and/or workmanship, PST will repair it or, at our option, replace it at no charge to you.

This warranty applies to all monitors, analyzers and sensors purchased worldwide.

8.2 Limitations

Analytical Industries Inc. will not pay for: loss of time; inconvenience; loss of use of your Analytical Industries Inc. analyzer or property damage caused by your Analytical Industries Inc. analyzer or its failure to work; any special, incidental or consequential damages; or any damage resulting from alterations, misuse or abuse; lack of proper maintenance; unauthorized repair or modification of the analyzer; affixing of any attachment not provided with the analyzer or other failure to follow the user manual.

US Customers only: Some states and provinces do not allow limitations on the duration of an implied warranty or the exclusion or limitation of special, incidental or consequential damages, in this case, these exclusions may not apply. This warranty gives you specific legal rights. You may have other rights, which vary between states and provinces.

8.3 Exclusions

This warranty does not cover installation; defects resulting from accidents; damage while in transit to our service location; damage resulting from alterations, misuse or abuse; lack of proper maintenance;

unauthorized repair or modification of the analyzer; affixing of any label or attachment not provided with the analyzer; fire, flood, or acts of God; or other failure to follow the User Manual.

8.4 Service

For queries related to service and warranty, please contact your local Process Sensing Technologies office, sales partner or supplier.

Offices are listed at ProcessSensing.com or email oxygen@processsensing.com.



9 Appendices

Appendix A - Technical Specifications

Sensor				
Electrochemical	ppm		%	
Model Number	GPR-12-333 GPR-12-333-LD GPR-12-333-H	XLT-12-333 XLT-12-333-LD	GPR-11-60 GPR-11-60-LD	XLT-11-24 XLT-11-24-LD
Measuring Range	0...10, 0...100, 0...1000 ppm _v , 0...1 % 0...25 % (calibration only)		0...1, 0...5, 0...10, 0...25 %	
Output Resolution	0.01 ppm _v		0.001 %	
Lower Detection Limit (LDL)	0.05 ppm _v		0.01 %	
Sample Flow Rate (application dependent)	1...2 SCFH (0.5...1 LPM)			
Pressure Range	5...30 psi (0.4...2.1 bar)			
Response Time (T90)	< 2 minutes		< 30 seconds	
Operating Temperature Range	+5 °C...+45 °C (+41 °F...+113 °F)	-10 °C...+45 °C (+14 °F...+113 °F)	+5 °C...+45 °C (+41 °F...+113 °F)	-10 °C...+45 °C (+14 °F...+113 °F)
Humidity	0...80 %rh non-condensing			
Life Expectancy (application dependent)	24 months in 1000 ppm _v		60 months in air	24 months in air
Calibration Interval (application dependent)	30 days			
Analyzer				
Electrical				
Display	LCD			
Output Signal	4...20 mA			
Power Supply	18...24 V DC			
Maximum Power Consumption	1.8 W			
Mechanical				
Ingress Protection	NEMA 3R			
Analyzer Housing Material	Fiberglass and painted aluminum			
Mounting	Wall / vertical surface			
Compliance				
Complies with EMC Directive: 2014/30/EU				

Appendix B - Hazardous Area Certification

Region	Certification details	Standards
Europe	 ATEX / UKCA II 1 G Ex ia IIC T4 Ga T _{amb} (-20 °C...+50 °C)	EN 60079-0:2018 EN 60079-1:2014 EN 60079-11:2012
North America/Canada	 cMETus Class I, Div 1, Groups A, B, C & D, T4 Class I, Zone 0, AEx ia IIC T4 Ga, Ex ia IIC T4 Ga T _{amb} (-20 °C...+50 °C)	UL 60079-0:2019 (R2020) UL 60079-1:2020 UL 60079-11:2013 (R2018) UL 1203:2022 UL 61010-1:2019 CSA C22.2 No. 60079-0:2019 CSA C22.2 NO. 60079-1:16 (R2021) CSA C22.2 No. 60079-11:2014 (R2018) CSA C22.2 NO. 30:20 CSA C22.2 No. 61010-1:2017
International	 IECEx Ex ia IIC T4 Ga T _{amb} (-20 °C...+50 °C)	IEC 60079-0:2017 IEC 60079-1:2014 IEC 60079-11:2011

Appendix C - Safety Data Sheet



Analytical Industries Inc.

A PST Brand

Safety Data Sheet (KOH)

I. Product Identification

Product Name: Oxygen Sensor (Series AII, GPR, PSR, Private Label derivations)
Product Use: Oxygen Sensors
Manufacturer: Analytical Industries Inc.
Address: 2855 Metropolitan Place, Pomona, CA 92767 USA
Contact Information: Tel: 909-392-6900, Fax: 909-392-3665, email: info@aai1.com
Emergency Number:

Date Prepared: January 1, 1995
Date Revised: January 31, 2023

II. Hazardou(s) Identification

GHS Classification:

Lead (Pb)

Health

Acute Toxicity- Category (Inhalation)
 Acute Toxicity- Category 4 (oral/dermal)
 Carcinogenic- Category 2ty
 Reproductive/Developmental- Category 2
 Target organ Toxicity (Repeated) Category 2

Environmental

Acute Aquatic Toxicity-Cat
 Chronic Aquatic Toxicity-Category 1

Physical

NA

Potassium Hydroxide (KOH)

Health

Corrosive to Metal- Category 1
 Acute Toxicity- Category 4 (oral)
 Skin Corrosion-Category 1A
 Serious Eye Damage-Category 1

Environmental

Acute Aquatic Toxicity-Cat

Physical

NA

GHS Labels:

Potassium Hydroxide (KOH)

Symbols:



Hazardous Statements

- Danger
- May be corrosive to metal
- Harmful if swallowed
- Causes severe skin burns and eye damage
- Harmful to aquatic life

Precautionary Statements

- Wash skin thoroughly after handling.
- Do not eat, drink or smoke when using this product.
- Avoid release to the environment.
- Wear protective gloves/ protective clothing/ eye protection/ face protection.
- IF SWALLOWED: Call a POISON CENTER or doctor/ physician if you feel unwell.
- IF SWALLOWED: Rinse mouth. Do NOT induce vomiting.
- IF ON SKIN (or hair): Remove/Take off immediately all contaminated clothing. Rinse skin with water/ shower.
- IF INHALED: Remove victim to fresh air and keep at rest in a position comfortable for breathing.
- IF IN EYES: Rinse cautiously with water for several minutes. Remove contact lens if present and easy to do. Continue rinsing. Immediately call a POISON CENTER or doctor/ physician.
- Wash contaminated clothing before reuse.
- Absorb spillage to prevent material damage.
- Store in corrosive resistant stainless steel container with a resistant inner liner.
- Dispose of contents/ container to an approved waste disposal plant.

GHS Labels:

Lead (Pb)

**Analytical Industries Inc.**

A PST Brand

Safety Data Sheet (KOH)**Symbols:****Hazardous Statements**

- Warning !
- Harmful if swallowed
- Suspected of causing cancer.
- Suspected of damaging fertility or the unborn child.
- May cause damage to organs through prolonged or repeated exposure.
- Very toxic to aquatic life with long lasting effects.

Precautionary Statements

- If breathed in, move person into fresh air. In not breathing, give artificial respiration. Consult a physician.
- In case of skin contact, wash off with soap and plenty of water.
- In case of eye contact, flush eyes with water as a precaution.
- If swallowed, rinse mouth with water.

III. Composition /Information on Ingredients

Material	C.A.S. #	Weight %	GHS Classification	Notes
Lead (Pb)	7439-92-1	50-75	Carc 1A;H350 Aquatic Acute 1:H400	Substance classified with a health & Environmental hazard. Substance with a work place limit
Potassium Hydroxide (KOH)	1310-58-3	1.0-10	Acute Tox. 4; H302 Skin Corr.1A; H314	Substance classified with a health & Environmental hazard. Substance with a work place limit.

IV. First Aid Measures**4.1. Description of aid measures****General:**

- In all cases of doubt, or when symptoms persist, seek medical attention. Never give anything by mouth to an unconscious person.

Inhalation:

- Remove to fresh air, keep patient warm and at rest. If breathing is irregular or stopped, give artificial respiration. If unconscious place in the recovery position and obtain immediate

Eyes:

- Irrigate copiously with clean water for at least 15 minutes, holding the eyelids apart and seek medical attention.

Skin:

- Remove contaminated clothing. Wash skin thoroughly with soap and water or use a recognized skin cleanser.

Ingestion:

- Do NOT induce vomiting. Rinse mouth and slowly drink several glasses of water. Call a physician. Do NOT give anything by mouth to an unconscious or

4.2. Most important symptoms and effects, both acute and delayed

- The most important known symptoms and effects are described in the labelling (see section II) and/or in section XI

V. Fire-Fighting Measures**5.1. Extinguishing media**

- Use standard fire fighting media on surrounding materials including water spray, foam, and carbon dioxide. (Do not use dry chemical extinguisher

5.2. Special hazards arising from the substance or mixture

- Lead Oxides.

5.3. Advice for fire-fighters

- Wear self-contained breathing apparatus for firefighting if necessary.



Analytical Industries Inc.

A PST Brand

Safety Data Sheet (KOH)

5.4. Further Information

- Gives off hydrogen by reaction with metals.

VI. Accidental release measures

Note: The Oxygen sensor contains a strong basic solution encapsulated in a plastic housing. Under normal operating conditions the solution (electrolyte) is never exposed. In case of a leak please observe the following instructions:

6.1. Personal precautions, protective equipment and emergency procedures

- Use appropriate personal protective equipment. Avoid dust formation. Avoid breathing vapors, mist or gas. Ensure adequate ventilation. Evacuate personnel to safe areas. Avoid breathing dust. For personal protection see section

6.2. Environmental precautions

- Do not allow spills to enter drains or waterways. Use good personal hygiene practices. Wash hands before eating, drinking, smoking or using toilet. Promptly remove soiled clothing and wash thoroughly before reuse.

6.3. Methods and material for containment and cleaning up

- Contain spillage. Neutralize spill with soda ash or lime. Carefully place material into clean dry contain and cover. Flush spill area with water. Avoid creating dust.

VII. Handling and storage

7.1. Precautions for safe handling

- Under normal circumstances the lead anode and potassium hydroxide electrolyte are sealed inside the oxygen sensor which is then sealed in a polyethylene bag and placed in a cardboard box for shipment) and do not present a health hazard. The following guidelines are provided in the event an oxygen sensor leaks
- Before opening the bag containing the sensor cell, check the sensor cell for leakage. If the sensor cell leaks, do not open the bag. If there is liquid around the cell while in the instrument, put on gloves and eye protection before removing the

7.2. Conditions for safe storage, including any incompatibilities

- Store sensors in a cool, dry and well-ventilated places. Exercise due caution to prevent damage to or leakage from the container. Keep containers closed when

7.3. Specific end use(s)

- Apart from the uses mentioned in section I no other specifies are stipulated.

VIII. Exposure Controls/Personal Protection

8.1. Control parameters

Exposure

CAS No.	Ingredient	Source	Value
0001310-58-3	Potassium hydroxide	OSHA ACGIH NIOSH Supplier	No Establish Limits Ceiling: 2mg/m ³ Ceiling: 2mg/m ³ No Establish Limits
007439-92-1	Lead (Pb)	OSHA ACGIH NIOSH Supplier	(1910.1025)TWA 0.050mg/m ³ TWA:0.05 mg/m ³ R,2B,2A TWA (8 Hour)0.050 mg/m ³ No Establish Limits

Carcinogen Data

CAS No.	Ingredient	Source	Value
0001310-58-3	Potassium hydroxide	OSHA NTP IARC	Select Carcinogen: No Known: No; Suspected: No Group 1: No; Group 2a: No; Group 2b: No; Group 3: No; Group 4: No;
007439-92-1	Lead (Pb)	OSHA	Select Carcinogen: Yes

**Analytical Industries Inc.**

A PST Brand

Safety Data Sheet (KOH)

NTP Known: No; Suspected: Yes
 Group 1: No; Group 2a: No;
 IARC Group 2b: Yes; Group 3: No;
 Group 4: No;

8.2. Exposure controls
Respiratory

- If workers are exposed to concentrations above the exposure limit they must use the appropriate, certified respirators.

Eyes

- Chemical splash goggles

Skin

- Apron, face shield Wear gloves. Gloves must be resistant to corrosive materials. Nitrile or PVC gloves are suitable. Do not use cotton or leather gloves.

Engineering Controls

- Provide adequate ventilation. Where reasonably practicable this should be achieved by the use of local exhaust ventilation and good general extraction. If these are not sufficient to maintain concentrations of particulates and any vapor below occupational exposure limits suitable respiratory protection must be worn.

Other Work Practices

- Use good personal hygiene practices. Wash hands before eating, drinking, smoking or using toilet. Promptly remove soiled clothing and wash thoroughly

IX. Physical / Chemical Characteristics**9.1 Information on basic physical and chemical properties****Material / Component:****Lead (Pb) - Anode****Potassium Hydroxide (KOH) - Electrolyte****Appearance**

Article Solid

Form: Liquid; **Color:** Clear Translucent**Odor**

None

None

Odor threshold

Not Measured

Not Measured

pH

Not Measured

>13

Melting point / freezing point

>328° C

Not Measured

Initial boiling point and boiling range

>1320° C

Not Measured

Flash Point

Not Measured

>100° C

Evaporation rate (Ether = 1)

Not Measured

Not Measured

Flammability (solid, gas)

Not Applicable

Not Measured

Upper/lower flammability or explosive limits

Not Measured

Not Measured

Vapor pressure

Not Measured

Not Measured

Vapor Density

Not Measured

Not Measured

Specific Gravity

Not Measured

Not Measured

Solubility in Water

Insoluble

100% (Water based solution)

Partition coefficient n-octanol/water (Log Kow)

Not Measured

Not Measured

Auto-ignition temperature

Not Measured

Not Measured

Decomposition temperature

Not Measured

Not Measured

Viscosity (cSt)

Not Measured

Not Measured

9.2. Other information

No other relevant information.

X. Stability and Reactivity**10.1. Reactivity**

- Hazardous Polymerization will not occur

10.2. Chemical stability

- Stable under normal circumstances

10.3. Possibility of hazardous reactions

- Incompatible with strong oxidizers, leather and halogenated compounds. Product will react with 'soft' metals such as aluminum, tin, magnesium, and zinc



Analytical Industries Inc.

A PST Brand

Safety Data Sheet (KOH)

10.4. Conditions to avoid

releasing flammable hydrogen gas.

- Excessive heat and open flame.

10.5. Incompatible materials

- Aluminum, organic materials, acid chlorides, acid anhydrides, magnesium, copper. Avoid contact with acids and hydrogen peroxide >52%

10.6. Hazardous decomposition products

- Toxic fumes.

XI. Toxicological Information

11.1 Information on toxicological effects (Potassium Hydroxide)

Acute toxicity

- LD50 Oral - Rat- 333mg/kg
- Inhalation : no data available
- Dermal: no data available

Skin Corrosion/irritation

- Skin Rabbit- Severe skin irritation 24 h

Serious eye damage/eye irritation

- Eyes Rabbit- Corrosive to eyes (OECD Test Guideline 405)

Respiratory or skin sensitization

- No Data Available

Germ cell mutagenicity

- No Data Available

Carcinogenicity

IARC • No component of this product presents at levels greater than or equal to 0.1% is identified as probable, possible or confirmed human carcinogen by IARC.

ACGIH • No component of this product presents at levels greater than or equal to 0.1% is identified as a carcinogen or potential carcinogen by ACGIH.

NTP • No component of this product presents at levels greater than or equal to 0.1% is identified as a known or anticipated carcinogen by NTP

OSHA • No component of this product presents at levels greater than or equal to 0.1% is identified as a carcinogen or potential carcinogen by OSHA

Reproductive toxicity

- No Data Available

Specific target organ toxicity-single exposure

- No Data Available

Specific target organ toxicity-repeated exposure

- No Data Available

Additional information

- RTECS:TT2100000

11.2 Information on toxicological effects (Lead)

Acute toxicity

- Inhalation : no data available
- Dermal: no data available

Skin Corrosion/irritation

- No Data Available

Serious eye damage/eye irritation

- No Data Available

Respiratory or skin sensitization

- No Data Available

Germ cell mutagenicity

- Rat - Cytogenetic analysis



Analytical Industries Inc.

A PST Brand

Safety Data Sheet (KOH)

Carcinogenicity

- Limited evidence of carcinogenicity in animal studies
- IARC** • 2B-Group 2B. Possibly carcinogenic to humans (Lead)
- NTP** • Reasonably anticipated to be a human carcinogen (Lead)
- OSHA** • 1910.1025 (Lead)

Reproductive toxicity

- Suspected human reproductive toxicant
- Rat-Inhalation: Effects on Newborn; Biochemical metabolic
- Rat-Oral: Effects on Newborn; Behavioral
- Mouse-Oral: Effect on Fertility: Female fertility index (e.g., # females pregnant per # sperm positive females; # females pregnant per # females mated). Effects on Fertility: Pre-implantation mortality (e.g., reduction in number of implants per female; total number of implants per corpora lutea).

Development Toxicity

- Rat-Inhalation: Effects on Embryo or Fetus: Fetotoxicity (except death, e.g., stunted fetus). Specific Developmental Abnormalities: Blood and lymphatic system (including spleen and marrow).
- Rat-Oral: Specific Developmental Abnormalities: Blood and lymphatic system (including spleen and marrow). Effects on Newborn: Growth statistics (e.g.,
- Rat-Oral: Effects on Embryo or Fetus: Fetotoxicity (except death, e.g., stunted fetus). Effects on Embryo or Fetus: Fetal death.
- Mouse-Oral: Effects on Embryo or Fetus: Fetotoxicity (except death, e.g., stunted fetus). Effects on Embryo or Fetus: Fetal death.

Specific target organ toxicity – single exposure

- No Data Available

Specific target organ toxicity – repeated exposure

- May cause damage to organs through prolonged or repeated exposure.

Aspiration hazard

- No Data Available

Additional Information

- RTECS: OF7525000

XII. Ecological Information

12.1. Toxicity

Very toxic to aquatic life

Aquatic Ecotoxicity

Ingredient	96 hr. LC50 fish, mg/l	48 hr. EC50 crustacea, mg/l	ErC50 algae, mg/l
Lead Compounds (as Pb) - (7439-92-1)	0.44, Cyprinus carpio	4.40, Daphnia magna	0.25 (72 hr.), Scenedesmus subspicatus
Potassium hydroxide. - (1310-58-3)	Not Available	Not Available	Not Available

12.1. Persistence and degradability

- There is no data available on the preparation itself.

12.3. Bioaccumulative potential

- Not Measured

12.4. Mobility in soil

- No Data Available

12.5. Result of PBT and vPvB assessment

- This Product contains no PBT and vPvB chemicals.

12.6. Other adverse effects

- Lead is bioaccumulative in most aquatic life and mammals. It is highly mobile as lead dust or fume, yet forms complexes with organic material which limits its

XIII. Disposal Considerations



Analytical Industries Inc.

A PST Brand

Safety Data Sheet (KOH)

13.1. Waste treatment methods

- Do not allow into drains or water courses. Wastes and emptied containers should be disposed of in accordance with regulations made under the Control of Pollution Act and the Environmental Protection Act.
- Using information provided in this data sheet advice should be obtained from the Waste Regulation Authority, whether the special waste regulations apply.

XIV. Transport Information

DOT:

- Regulated. Refer to Small Quantity Exceptions: 49 CFR 173.4
- UN3266, Corrosive liquid, basic, inorganic, n.o.s., (potassium hydroxide, lead), 8, II NOTE: This description is used for shipping purposes when not using Analytical Industries Inc. US DOT Approval.
- UN3363, Dangerous Goods in Machinery or Dangerous Goods in Apparatus, 9. NOTE: This description is used when shipping under the US DOT Approval.

IATA:

- Regulated. Meets criteria for IATA Dangerous Goods in Excepted Quantities, Secti

Environmental hazards IMDG

- Marine Pollutant: Yes (Lead Compounds (as Pb))

XV. Regulatory Information

Regulatory Overview

- The regulatory data in Section 15 is not intended to be all-inclusive, only selected regulations are represented.

Toxic Substance Control Act (TSCA)

- All components of this material are either listed or exempt from listing on the TSCA Inventory

WHMIS Classification

- D2A E

US EPA Tier II Hazards

Fire: No
Sudden Release of Pressure: No
Reactive: No
Immediate (Acute): Yes
Delayed (Chronic): Yes

EPCRA 311/312 Chemicals and RQs (lbs.):

- Lead Compounds (as Pb) (10.00)
- Potassium hydroxide. (1,000.00)

EPCRA 302 Extremely Hazardous :

- (No Product Ingredients Listed)

EPCRA 313 Toxic Chemicals:

- Lead Compounds (as Pb)

Proposition 65 - Carcinogens (>0.0%):

- Lead Compounds (as Pb)

Proposition 65 - Developmental Toxins (>0.0%):

- Lead Compounds (as Pb)

Proposition 65 - Female Repro Toxins (>0.0%):

- Lead Compounds (as Pb)

Proposition 65 - Male Repro Toxins (>0.0%):

- Lead Compounds (as Pb)

N.J. RTK Substances (>1%):

- Lead Compounds (as Pb)
- Potassium hydroxide.

XVI. Other Information

The information and recommendations contained herein are based upon data believed to be correct. However, no guarantee or warranty of

***Analytical Industries Inc.***

A PST Brand

Safety Data Sheet (KOH)

any kind, expressed or implied, is made with respect to the information contained herein. We accept no responsibility and disclaim all liability for any harmful effects which may be caused by exposure to our products. Customers/users of this product must comply with all applicable health and safety laws, regulations, and orders.

H302 Harmful if swallowed.

H314 Causes severe skin burns and eye damage.

H350 May cause cancer.

H400 Very toxic to aquatic life.

This is the first version in the GHS SDS format. Listings of changes from previous versions in other formats are not

All chemicals may pose unknown hazards and should be used with caution. While the information contained in this Material Safety Data Sheet is believed to be correct and is offered for your information, consideration and investigation, Analytical Industries Inc assumes no responsibility of the completeness or accuracy of the information contained herein.

End of Document


Appendix D - Controlled Drawings

4		3		2		1																																			
THE LOOP POWERED GAS ANALYZER IS NOT CAPABLE OF WITHSTANDING THE 500V INSULATION DIELECTRIC STRENGTH TEST REQUIRED BY IEC 60079-11. THIS SHALL BE TAKEN INTO ACCOUNT WHEN INSTALLING THE EQUIPMENT. THE INSTALLATION MUST COMPLY WITH THE INSTALLATION PRACTICES OF THE COUNTRY OF USE. I.e. THE NATIONAL ELECTRICAL CODE ANSI/NFPA 70 AND THE CANADIAN ELECTRICAL CODE CSA C22.1.				PRODUCT MODEL NUMBER: GPR-1500, GPR-2500 EQUIPMENT TYPE ID: LOOP POWERED GAS ANALYZER CERTIFICATE NUMBER: E115647 DIVISION SYSTEM MARKING: Class I Div 1 Groups ABCD, T4 ZONE SYSTEM MARKING: Class I Zone 0 AEx ia IIC T4 Ga IEC / CANADA: Ex ia IIC T4 Ga				<table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <th colspan="5">RÉVISIONS</th> </tr> <tr> <th>ZONE</th> <th>REV.</th> <th>DESCRIPTION</th> <th>DATE</th> <th>APPROVED</th> </tr> <tr> <td> </td> <td> </td> <td> </td> <td> </td> <td> </td> </tr> </table>		RÉVISIONS					ZONE	REV.	DESCRIPTION	DATE	APPROVED																						
RÉVISIONS																																									
ZONE	REV.	DESCRIPTION	DATE	APPROVED																																					
HAZARDOUS LOCATION ← → NON-HAZARDOUS LOCATION																																									
HAZARDOUS AREA INSTALLATIONS 1. THERE IS ONLY ONE CONNECTION WHICH IS INTRINSICALLY SAFE. ITS PARAMETER TABLE IS: <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>GROUP</th> <th>Ui (V)</th> <th>Ii (mA)</th> </tr> </thead> <tbody> <tr> <td>B or IIC</td> <td rowspan="3">28</td> <td rowspan="3">93</td> </tr> <tr> <td>C or IIB</td> </tr> <tr> <td>D or IIA</td> </tr> </tbody> </table> OTHER PARAMETERS ARE DETERMINED BY THE CONNECTED EQUIPMENT 2. WARNING: SUBSTITUTION OF COMPONENTS MAY IMPAIR INTRINSIC SAFETY 3. ALL CABLE MUST BE SHIELDED TO GROUND AT CUSTOMER SIDE.				GROUP	Ui (V)	Ii (mA)	B or IIC	28	93	C or IIB	D or IIA	<table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td colspan="2" style="font-size: small;">UNLESS OTHERWISE SPECIFIED:</td> <td>NAME</td> <td>DATE</td> <td rowspan="5" style="text-align: center; vertical-align: middle;"> ANALYTICAL INDUSTRIES INC. TITLE: LOOP POWERED GAS ANALYZER SYSTEM DRAWING SIZE DWG. NO. B A-5594-EX SCALE: WEIGHT: SHEET 1 OF 2 </td> </tr> <tr> <td colspan="2" style="font-size: x-small;">DIMENSIONS ARE IN INCHES TOLERANCES: FRACTIONS: 1/16" ANGULAR: MACH 1/2 BEND: 90° TWO PLACE DECIMAL: 0.05 THREE PLACE DECIMAL: 0.003</td> <td>DRAWN</td> <td>07/10/23</td> </tr> <tr> <td colspan="2" style="font-size: x-small;">INTERPRET GEOMETRIC TOLERANCING PER: ANSI Y14.5</td> <td>CHECKED</td> <td> </td> </tr> <tr> <td colspan="2" style="font-size: x-small;">MATERIAL:</td> <td>ENG APPR.</td> <td> </td> </tr> <tr> <td colspan="2" style="font-size: x-small;">FINISH:</td> <td>MFG APPR.</td> <td> </td> </tr> <tr> <td colspan="2" style="font-size: x-small;">DO NOT SCALE DRAWING</td> <td colspan="2" style="font-size: x-small;">COMMENTS:</td> <td> </td> </tr> </table>				UNLESS OTHERWISE SPECIFIED:		NAME	DATE	ANALYTICAL INDUSTRIES INC. TITLE: LOOP POWERED GAS ANALYZER SYSTEM DRAWING SIZE DWG. NO. B A-5594-EX SCALE: WEIGHT: SHEET 1 OF 2	DIMENSIONS ARE IN INCHES TOLERANCES: FRACTIONS: 1/16" ANGULAR: MACH 1/2 BEND: 90° TWO PLACE DECIMAL: 0.05 THREE PLACE DECIMAL: 0.003		DRAWN	07/10/23	INTERPRET GEOMETRIC TOLERANCING PER: ANSI Y14.5		CHECKED		MATERIAL:		ENG APPR.		FINISH:		MFG APPR.		DO NOT SCALE DRAWING		COMMENTS:		
GROUP	Ui (V)	Ii (mA)																																							
B or IIC	28	93																																							
C or IIB																																									
D or IIA																																									
UNLESS OTHERWISE SPECIFIED:		NAME	DATE	ANALYTICAL INDUSTRIES INC. TITLE: LOOP POWERED GAS ANALYZER SYSTEM DRAWING SIZE DWG. NO. B A-5594-EX SCALE: WEIGHT: SHEET 1 OF 2																																					
DIMENSIONS ARE IN INCHES TOLERANCES: FRACTIONS: 1/16" ANGULAR: MACH 1/2 BEND: 90° TWO PLACE DECIMAL: 0.05 THREE PLACE DECIMAL: 0.003		DRAWN	07/10/23																																						
INTERPRET GEOMETRIC TOLERANCING PER: ANSI Y14.5		CHECKED																																							
MATERIAL:		ENG APPR.																																							
FINISH:		MFG APPR.																																							
DO NOT SCALE DRAWING		COMMENTS:																																							


4		3		2		1																																			
L'ANALYSEUR DE GAZ ALIMENTÉ PAR LA BOUCLE DE COURANT N'EST PAS CAPABLE DE RÉSISSER À L'ESSAI DE RIGIDITÉ DIÉLECTRIQUE DE 500V REQUIS PAR LA NORME IEC 60079-11. IL CONVIENT D'EN TENIR COMPTE LORS DE L'INSTALLATION DE L'ÉQUIPEMENT. L'INSTALLATION DOIT ÊTRE CONFORME AUX PRATIQUES D'INSTALLATION DU PAYS D'UTILISATION, C'EST-À-DIRE LE CODE ÉLECTRIQUE NATIONAL ANSI/NFPA 70 ET LE CODE ÉLECTRIQUE CANADIEN CSA C22.1.				NUMÉRO DE MODÈLE DU PRODUIT : GPR-1500, GPR-2500 TYPE D'ÉQUIPEMENT ID : LOOP POWERED GAS ANALYZER NUMÉRO DE CERTIFICAT : E115647 MARQUAGE DU SYSTÈME DE DIVISION : Class I Div 1 Groups ABCD, T4 MARQUAGE DU SYSTÈME DE ZONES : Class I Zone 0 AEx ia IIC T4 Ga IEC / CANADA: Ex ia IIC T4 Ga				<table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <th colspan="5">RÉVISIONS</th> </tr> <tr> <th>ZONE</th> <th>REV.</th> <th>DESCRIPTION</th> <th>DATE</th> <th>APPROUVÉE</th> </tr> <tr> <td> </td> <td> </td> <td> </td> <td> </td> <td> </td> </tr> </table>		RÉVISIONS					ZONE	REV.	DESCRIPTION	DATE	APPROUVÉE																						
RÉVISIONS																																									
ZONE	REV.	DESCRIPTION	DATE	APPROUVÉE																																					
ZONE DANGEREUSE ← → EMBLACEMENT NON DANGEREUX																																									
INSTALLATIONS EN ZONE DANGEREUSE 1. IL N'Y A QU'UNE SEULE CONNEXION QUI SOIT INTRINSÈQUEMENT SÛRE. SON TABLEAU DE PARAMÈTRES EST LE SUIVANT: <table border="1" style="width: 100%; border-collapse: collapse;"> <thead> <tr> <th>GROUPE</th> <th>Ui (V)</th> <th>Ii (mA)</th> </tr> </thead> <tbody> <tr> <td>B ou IIC</td> <td rowspan="3">28</td> <td rowspan="3">93</td> </tr> <tr> <td>C ou IIB</td> </tr> <tr> <td>D ou IIA</td> </tr> </tbody> </table> LES AUTRES PARAMÈTRES SONT DÉTERMINÉS PAR L'ÉQUIPEMENT CONNECTÉ 2. AVERTISSEMENT : LA SUBSTITUTION DE COMPOSANTS PEUT NUIRE À LA SÉCURITÉ INTRINSÈQUE 3. TOUS LES CÂBLES DOIVENT ÊTRE BLINDÉS JUSQU'À LA TERRE PAR LE CLIENT.				GROUPE	Ui (V)	Ii (mA)	B ou IIC	28	93	C ou IIB	D ou IIA	<table border="1" style="width: 100%; border-collapse: collapse;"> <tr> <td colspan="2" style="font-size: small;">SAUF INDICATION CONTRAIRE LES DIMENSIONS SONT: ENCHÈVRES EN POUCES, AVEC TOLÉRANCES: FRACTIONS: 1/16" ANGULAR: MACH 1/2 BEND: 90° DECIMALES: 4 VOS PLACES: 0.05 DECIMALES À TROIS PLACES: 0.003</td> <td>INOM</td> <td>DATE</td> <td rowspan="5" style="text-align: center; vertical-align: middle;"> ANALYTICAL INDUSTRIES INC. TITLE: SCHÉMA DU SYSTÈME D'ANALYSE DE GAZ ALIMENTÉ PAR UNE BOUCLE DE COURANT TAILLE DWG. NO. B A-5594-EX ÉCHELLE : POIDS : FICHE 1 SUR 2 </td> </tr> <tr> <td colspan="2" style="font-size: x-small;">INTERPRÉTER LE TOLÉRANCING GÉOMÉTRIQUE SELON: ANSI Y14.5</td> <td>TRÉ</td> <td>07/10/23</td> </tr> <tr> <td colspan="2" style="font-size: x-small;">MATERIAL:</td> <td>VÉRIFÉ</td> <td> </td> </tr> <tr> <td colspan="2" style="font-size: x-small;">FINISH:</td> <td>ENG APPR.</td> <td> </td> </tr> <tr> <td colspan="2" style="font-size: x-small;">NE PAS METTRE LE DRESS À L'ÉCHELLE</td> <td>MFG APPR.</td> <td> </td> </tr> <tr> <td colspan="2" style="font-size: x-small;">EXCERPT ET CONFIDENTIAL: LES INFORMATIONS CONTENUES DANS CE DRESS SONT LA PROPRIÉTÉ EXCLUSIVE DE ANALYTICAL INDUSTRIES INC. TOUTE RÉPÉTION NON PERMISE QU'ELLE SOIT SANS L'AUTORISATION ÉCRITE DE ANALYTICAL INDUSTRIES INC. ES INTRINSÈQUE</td> <td colspan="2" style="font-size: x-small;">COMMENTS:</td> <td> </td> </tr> </table>				SAUF INDICATION CONTRAIRE LES DIMENSIONS SONT: ENCHÈVRES EN POUCES, AVEC TOLÉRANCES: FRACTIONS: 1/16" ANGULAR: MACH 1/2 BEND: 90° DECIMALES: 4 VOS PLACES: 0.05 DECIMALES À TROIS PLACES: 0.003		INOM	DATE	ANALYTICAL INDUSTRIES INC. TITLE: SCHÉMA DU SYSTÈME D'ANALYSE DE GAZ ALIMENTÉ PAR UNE BOUCLE DE COURANT TAILLE DWG. NO. B A-5594-EX ÉCHELLE : POIDS : FICHE 1 SUR 2	INTERPRÉTER LE TOLÉRANCING GÉOMÉTRIQUE SELON: ANSI Y14.5		TRÉ	07/10/23	MATERIAL:		VÉRIFÉ		FINISH:		ENG APPR.		NE PAS METTRE LE DRESS À L'ÉCHELLE		MFG APPR.		EXCERPT ET CONFIDENTIAL: LES INFORMATIONS CONTENUES DANS CE DRESS SONT LA PROPRIÉTÉ EXCLUSIVE DE ANALYTICAL INDUSTRIES INC. TOUTE RÉPÉTION NON PERMISE QU'ELLE SOIT SANS L'AUTORISATION ÉCRITE DE ANALYTICAL INDUSTRIES INC. ES INTRINSÈQUE		COMMENTS:		
GROUPE	Ui (V)	Ii (mA)																																							
B ou IIC	28	93																																							
C ou IIB																																									
D ou IIA																																									
SAUF INDICATION CONTRAIRE LES DIMENSIONS SONT: ENCHÈVRES EN POUCES, AVEC TOLÉRANCES: FRACTIONS: 1/16" ANGULAR: MACH 1/2 BEND: 90° DECIMALES: 4 VOS PLACES: 0.05 DECIMALES À TROIS PLACES: 0.003		INOM	DATE	ANALYTICAL INDUSTRIES INC. TITLE: SCHÉMA DU SYSTÈME D'ANALYSE DE GAZ ALIMENTÉ PAR UNE BOUCLE DE COURANT TAILLE DWG. NO. B A-5594-EX ÉCHELLE : POIDS : FICHE 1 SUR 2																																					
INTERPRÉTER LE TOLÉRANCING GÉOMÉTRIQUE SELON: ANSI Y14.5		TRÉ	07/10/23																																						
MATERIAL:		VÉRIFÉ																																							
FINISH:		ENG APPR.																																							
NE PAS METTRE LE DRESS À L'ÉCHELLE		MFG APPR.																																							
EXCERPT ET CONFIDENTIAL: LES INFORMATIONS CONTENUES DANS CE DRESS SONT LA PROPRIÉTÉ EXCLUSIVE DE ANALYTICAL INDUSTRIES INC. TOUTE RÉPÉTION NON PERMISE QU'ELLE SOIT SANS L'AUTORISATION ÉCRITE DE ANALYTICAL INDUSTRIES INC. ES INTRINSÈQUE		COMMENTS:																																							

Appendix E - Mounting Information

GPR-x500

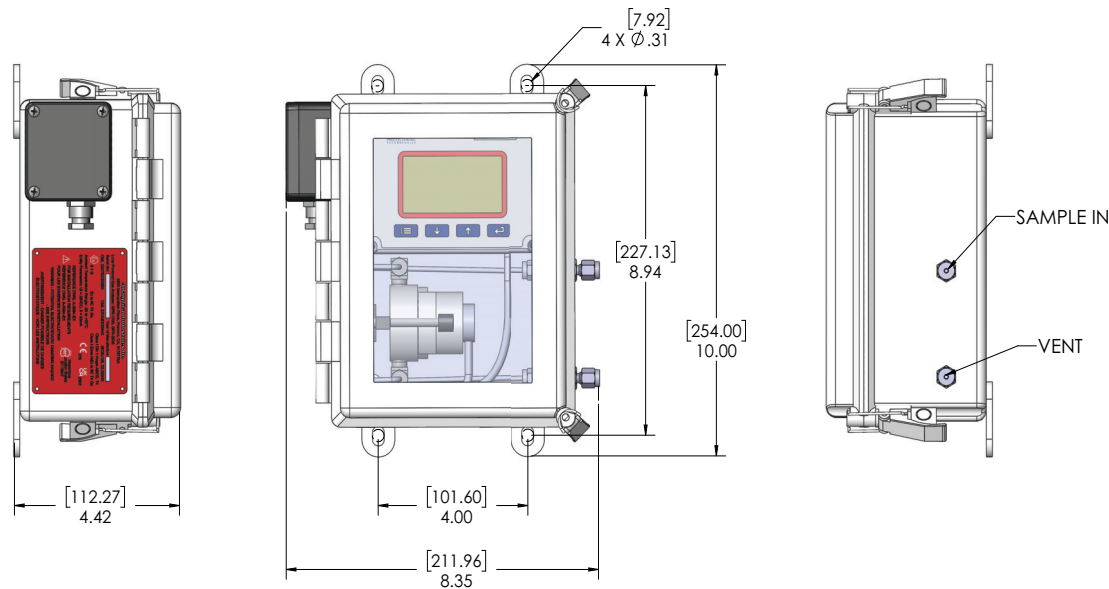

GPR-x500 with sample system

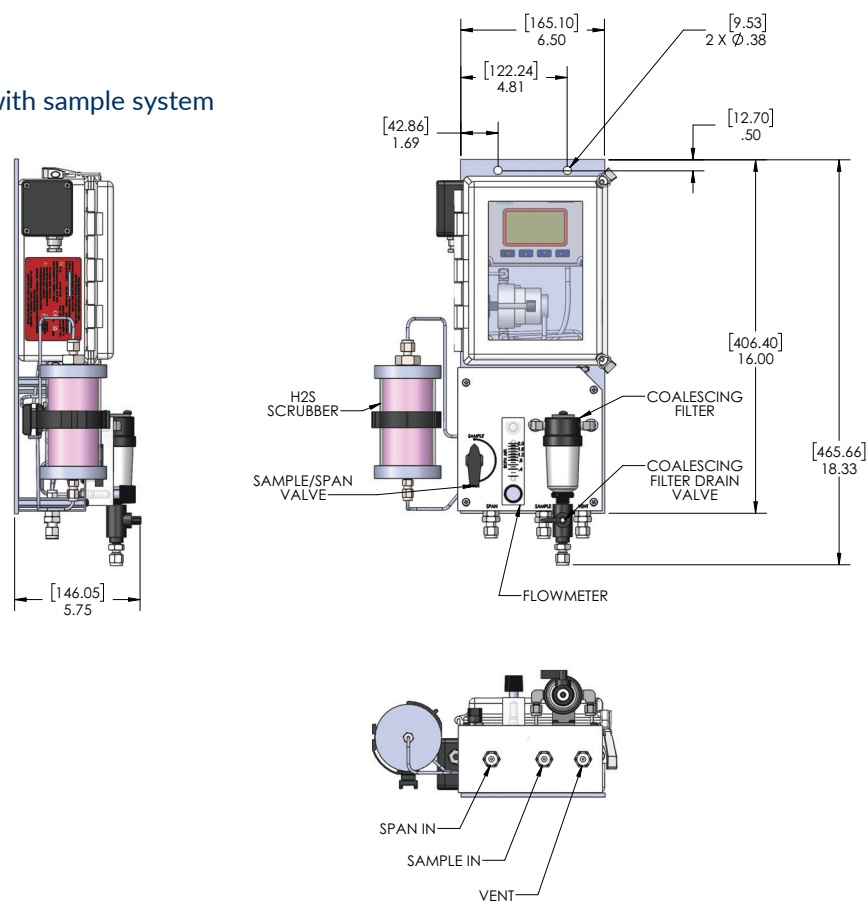

Appendix F - Menu Displays

MAIN MENU

➤ RANGE=AUTO
CALIBRATION
ALARMS=ON/OFF
SYSTEM
INFO

RANGE

➤ AUTO/FIXED
0-20 PPM
0-50 PPM
0-100 PPM
DEF RANGE=OFF

DEFAULT RANGE

➤ OFF/ON
0-10 PPM
0-100 PPM
0-1000 PPM
0-1%
0-25%
AUTO

CALIBRATION

SENSOR SN=20000123
SPAN CAL
ZERO CAL
CALIBRATION LOG
RESET CAL

ALARMS

➤ ALARMS=ON
ALARM 1
ALARM 2
LATCH VALVE
TONE ON/OFF

ALARM 1

ON / OFF
SETPOINT
MODE
DELAY
LATCHING
FAILSAFE

ALARM 2

ON / OFF
SETPOINT
MODE
DELAY
LATCHING
FAILSAFE

SYSTEM

➤ SECURITY
CALIBRATE 4-20mA
MODBUS=1
SIGNAL AVG=1
CLIPPING=ON/OFF
TIME=00:00
DATE FORM=MM/DD/YYYY

SECURITY

LOCK NOW
SET PASSCODE
AUTO LOCK

CALIBRATE 4-20 mA

ADJUST OUTPUT TO 4 mA
REF: 0

▲ ▼ EDIT

≡ ABORT

↵ 20 mA

MODBUS

➤ SLAVE ID=001
BAUD RATE=9600
PARITY
RESET COUNTERS
TOTAL
ERRORS
EXCEPT

INFO

UNIT ID=
ANA SN=000000000
PCB SN=000000000
FIRM=S1013 1.07
CONFIG=ACDC H2S-1

NOTE: The menu structure may vary depending on your configuration.

Appendix G - Spare Parts

Sensors	
GPR-12-333	ppm oxygen sensor
GPR-12-333-LD	ppm oxygen sensor for analyzer with liquid drain system
GPR-12-333-H	ppm oxygen sensor for He and H ₂ gases
XLT-12-333	ppm oxygen sensor for gases with < 0.5 % CO ₂ presence
XLT-12-333-LD	ppm oxygen sensor for gases with < 0.5 % CO ₂ presence and analyzer
	with liquid drain system
GPR-11-60	% oxygen sensor
GPR-11-60-LD	% oxygen sensor for analyzer with liquid drain system
XLT-11-24	% oxygen sensor for gases with < 0.5 % CO ₂ presence
XLT-11-24-LD	% oxygen sensor for gases with < 0.5 % CO ₂ presence and analyzer
	with liquid drain system
Operational Spares	
CHEM-1008-2	H ₂ S scrubber material (sampling system only, not LD)
FLTR-1037	Coalescing filter element (sampling system only, not LD)
BARR-1002	Intrinsically Safe remote barrier (B2 option only)
ORNG-1007	O-ring 3/32 x 1-3/8 x 1-9/16 Viton
Analyzer Hardware Spares	
B-2762-A-3-18	Sensor top housing assembly stainless steel

Appendix H - Rating Plate



Appendix I - Quality, Recycling, and Warranty Information

Aii is part of the Process Sensing Technologies (PST) Group. The PST Oxygen group of companies - Aii, Ntron and SST - comply with applicable national and international standards and directives.

Full information can be found on this website

<https://www.processsensing.com/en-us/resources/compliance/>

The compliance site contains information on the following directives:

- ATEX (equipment for explosive atmosphere, Europe)
- CE
- cMETus (electrical equipment for hazardous areas, North America)
- IECEx
- REACH (Registration, Evaluation, Authorization, and Restriction of Chemicals)
- Recycling policy
- RoHS (Restriction of Hazardous Substances in electrical and electronic equipment)
- UKCA
- WEEE (Waste Electrical and Electronic Equipment recycling).

This page is intentionally blank.

This page is intentionally blank.



ProcessSensing.com

Analytical Industries Incorporated (Aii) is part of the Process Sensing Technologies Group

©2024 Process Sensing Technologies
